



Healer Products Certificates of Analysis (COA)

Dear Healer Patron,

We are committed to producing high quality, clean, and accurately labeled cannabis products to help you feel your best. As you'll see in the following pages, we invest in the most thorough testing available in our region, not just for the content of medicinal components, but also for the absence of pesticides, toxic solvents, heavy metals, and microbiological contaminants.

To be transparent and earn your trust, our third-party laboratory certificates of analysis are attached.

Having previously owned and participated in a cannabis analytic laboratory for several years, I understand the inherent challenges related to reproducibility, calibration, and validation with peer laboratories. In the cannabis analytic industry, potency results are considered accurate within 10% deviation from the actual value. That's why after Healer performs its own internal analytics, we send samples of our bulk extracts and final products to at least one third-party lab, and sometimes two.

If you have any questions about the data on the following pages, we'd love to hear from you. Thank you for choosing Healer and taking a powerful step for your good health.

Sincerely,

Dr. Dustin Sulak

CANNABINOIDS

Cannabinoid	Concentration mg/ml
TOTAL	50.64
CBC	2.99
CBCA	
CBD	4.73
CBDA	2.31
CBDV	
CBDVA	
CBG	34.30
CBGA	5.76
CBL	
CBLA	
CBN	
CBNA	
Δ^8 -THC	
Δ^9 -THC	0.55
Δ^{10} -THC	
EXO-THC	
THCA	
THCV	
THCVA	
3 rd Party Tested By:	Nova Analytic Labs
3 rd Party Testing ID:	CBG.T.23.002-Cann NAL-230807-007

*<LOQ = Compound present in detectable amounts below the limit of quantitation for data reporting.

Product Type:

6:1 CBG:CBGA Tincture

Product Expiration Date:

August 15, 2025

COA Issue Date:

August 16, 2023

Ingredients:

Organic MCT Coconut Oil,
Organic Maine Hemp <0.3%
THC, Traces of Ethyl Alcohol
(Ethanol).

Strains:

White CBG, Stem Cell CBG,
Sour G, Forbidden V, Sour
Elektra, Suver Haze, Lifter,
Hawaiian Haze, Sour Space
Candy

Whole Plant Hemp CBG Drops

Batch ID: CBG.T.23.002



Healer

RESIDUAL SOLVENTS

TEST	RESULTS
Ethanol	Pass- 8190 ug/g (8.19 mg/g)
3 rd Party Tested By:	Nova Analytic Labs
3 rd Party Testing ID:	CBG.T.23.002 NAL-230808-038

*For full list of solvents see attached

MICROBIOLOGICAL CONTAMINANTS

TEST	RESULTS
Enterobacter	Pass-None Detected
Coliform	Pass-None Detected
Aerobic Bacteria	Pass-None Detected
Yeast and Mold	Pass-None Detected
Salmonella	Pass-None Detected
E.Coli	Pass-None Detected
3 rd Party Tested By:	Nova Analytic Labs
3 rd Party Testing ID:	CBG.T.23.002-Micro NAL-230808-035

HEAVY METALS

TEST	RESULTS
Arsenic	Pass-None Detected
Cadmium	Pass-None Detected
Lead	Pass-None Detected
Mercury	Pass-None Detected
3 rd Party Tested By:	Nova Analytic Labs
3 rd Party Testing ID:	H.21.001.D, H.22.004.D, H.23.006.A, H.23.006.D, H.22.005.A, H.22.007.A NAL-210507-007, NAL-220929-003, NAL-221107-003, NAL-221219-003, NAL-230721-019
Concentrated formula tested	

PESTICIDES

TEST	RESULT
Bifenthrin	Pass-None Detected
Cyfluthrin	Pass-None Detected
Daminozide	Pass-None Detected
Etoxazole	Pass-None Detected
Imazalil	Pass-None Detected
Myclobutanil	Pass-None Detected
Spiromesifen	Pass-None Detected
Trifloxystrobin	Pass-None Detected
3 rd Party Tested By:	Nova Analytic Labs
3 rd Party Testing ID:	H.21.001.D, H.22.004.D, H.23.006.A, H.23.006.D, H.22.005.A, H.22.007.A NAL-210702-015, NAL-220929-002, NAL-221107-004, NAL-221219-004, NAL-230721-018
Concentrated formula tested	

TERPENES

Terpene	Concentration mg/ml
TOTAL	2.770
PERCENT BY Wt	0.30%
β -Caryophyllene	1.120
α -Humulene	0.406
D-Limonene	
α -Pinene	
β -Myrcene	
β -Pinene	
Linalool	
Camphene	
α -Bisabolol	0.783
γ -Terpinene	
Terpinolene	
P-Cymene	
Isopulegol	
Guaiol	0.460
Cis-Nerolidol	
Eucalyptol	
Δ^3 -Carene	
Caryophyllene Oxide	
β -Ocimene	
α -Terpinene	
α -Ocimene	
Trans-Nerolidol	
3 rd Party Tested By:	Nova Analytic Labs
3 rd Party Testing ID:	CBG.T.23.002 NAL-230808-037

*<LOQ = Compound present in detectable amounts below the limit of quantitation for data reporting

Mycotoxins

TEST	RESULTS
Aflatoxins B1, B2, G1, G2	Pass-None Detected
Ochratoxin A	Pass- None Detected
3 rd Party Tested By:	Nova Analytic Labs
3 rd Party Testing ID:	CBG.T.23.002-Myco NAL-230808-036

3rd Party Lab
Results Attached




CERTIFICATE OF ANALYSIS

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

CBG.T.23.002-CANN2 (TINCTURE) // PRODUCED: AUG 07, 2023

CLIENT: HEALER HEMP LLC // BATCH: PASSED



BATCH NO.: CBG.T.23.002 ¹
MATRIX: TINCTURE ¹
DENSITY: 0.931 g/ml ²
SAMPLE ID: NAL-230807-007
COLLECTED ON: AUG 07, 2023
RECEIVED ON: AUG 07, 2023
SAMPLE SIZE: 2.600 G ¹
SAMPLED BY: ANNA KUPEL
RECEIVED BY: CJ LANGLEY
SERVING SIZE: 1 ML ²

CANNABINOID OVERVIEW

CBG: 34.3 mg/srv
CBGA: 5.76 mg/srv
TOTAL CANNABINOIDS: 50.6 mg/srv

¹ ENTERED BY CLIENT, ² ENTERED BY LAB

MANUFACTURER INFO

MANUFACTURER
 HEALER HEMP LLC
 119 ORION ST
 BRUNSWICK, MAINE 04011

LICENSE
 CGR26424
 MEDICINAL - CAREGIVER

BATCH RESULT: PASSED

POTENCY PASS

CAN.1: POTENCY & CANNABINOID PROFILE BY HPLC-UV PREPARATION: AUG 07, 2023 // ANALYSIS: AUG 07, 2023

ANALYTE	LIMIT	AMT	AMT	LOD/LOQ (mg/ml)	PASS/FAIL
CBC	0.321 %	2.99 mg/ml		0.0200/0.0996	N/A
CBCA	ND	ND		0.0200/0.0996	N/A
CBD	0.508 %	4.73 mg/ml		0.0200/0.0996	N/A
CBDA	0.248 %	2.31 mg/ml		0.0200/0.0996	N/A
CBDV	ND	ND		0.0200/0.0996	N/A
CBDVA	ND	ND		0.0200/0.0996	N/A
CBG	3.68 %	34.3 mg/ml		0.200/0.996	N/A
CBGA	0.619 %	5.76 mg/ml		0.0200/0.0996	N/A
CBL	ND	ND		0.0200/0.0996	N/A
CBLA	ND	ND		0.0200/0.0996	N/A
CBN	ND	ND		0.0200/0.0996	N/A
CBNA	ND	ND		0.0200/0.0996	N/A
Δ ⁸ -THC	ND	ND		0.0200/0.0996	N/A

ANALYTE	LIMIT	AMT	AMT	LOD/LOQ (mg/ml)	PASS/FAIL
Δ ⁸ -THCA		ND	ND	0.0200/0.0996	N/A
Δ ⁹ -THC	0.0585 %	0.545 mg/ml		0.0200/0.0996	N/A
Δ ¹⁰ -THC		ND	ND	0.0200/0.0996	N/A
EXO-THC		ND	ND	0.0200/0.0996	N/A
THCA		ND	ND	0.0200/0.0996	N/A
THCV		ND	ND	0.0200/0.0996	N/A
THCVA		ND	ND	0.0200/0.0996	N/A
TOTAL THC**	0.0585 %	0.545 mg/ml			N/A
TOTAL CBD**	0.725 %	6.75 mg/ml			N/A
CBD/SRV		4.73 mg			N/A
Δ ⁹ -THC/SRV		0.545 mg			N/A
TOTAL THC/SRV**		0.545 mg			N/A
TOTAL CBD/SRV**		6.75 mg			N/A

** TOTAL CBD = (CBDA X 0.877) + CBD

** TOTAL THC = (THCA X 0.877) + THC

Reported on an as received basis

1000 µg/g = 1 mg/g



AUTHORIZED BY:
 ZACHARY SMITH
 LABORATORY MANAGER, NOVA
 ANALYTIC LABS
 AUG 07, 2023

https://lims.tagleaf.com/coa/_xeVqkNZtCE

NOTES


ZACHARY SMITH
AUG 07, 2023

POTENCY & CANNABINOID PROFILE BY HPLC-UV
THE STANDARD LAB UNCERTAINTY FOR POTENCY IS 5% OF THE REPORTED VALUE.

** FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.*

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OCP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED, THIS CERTIFICATE OF ANALYSIS IS RELEVANT ONLY TO THOSE ITEMS TESTED. THE SAMPLE WAS PROVIDED TO THE LABORATORY FOR TESTING BY THE CLIENT AND THE SAMPLE WAS TESTED AS RECEIVED.

END OF REPORT

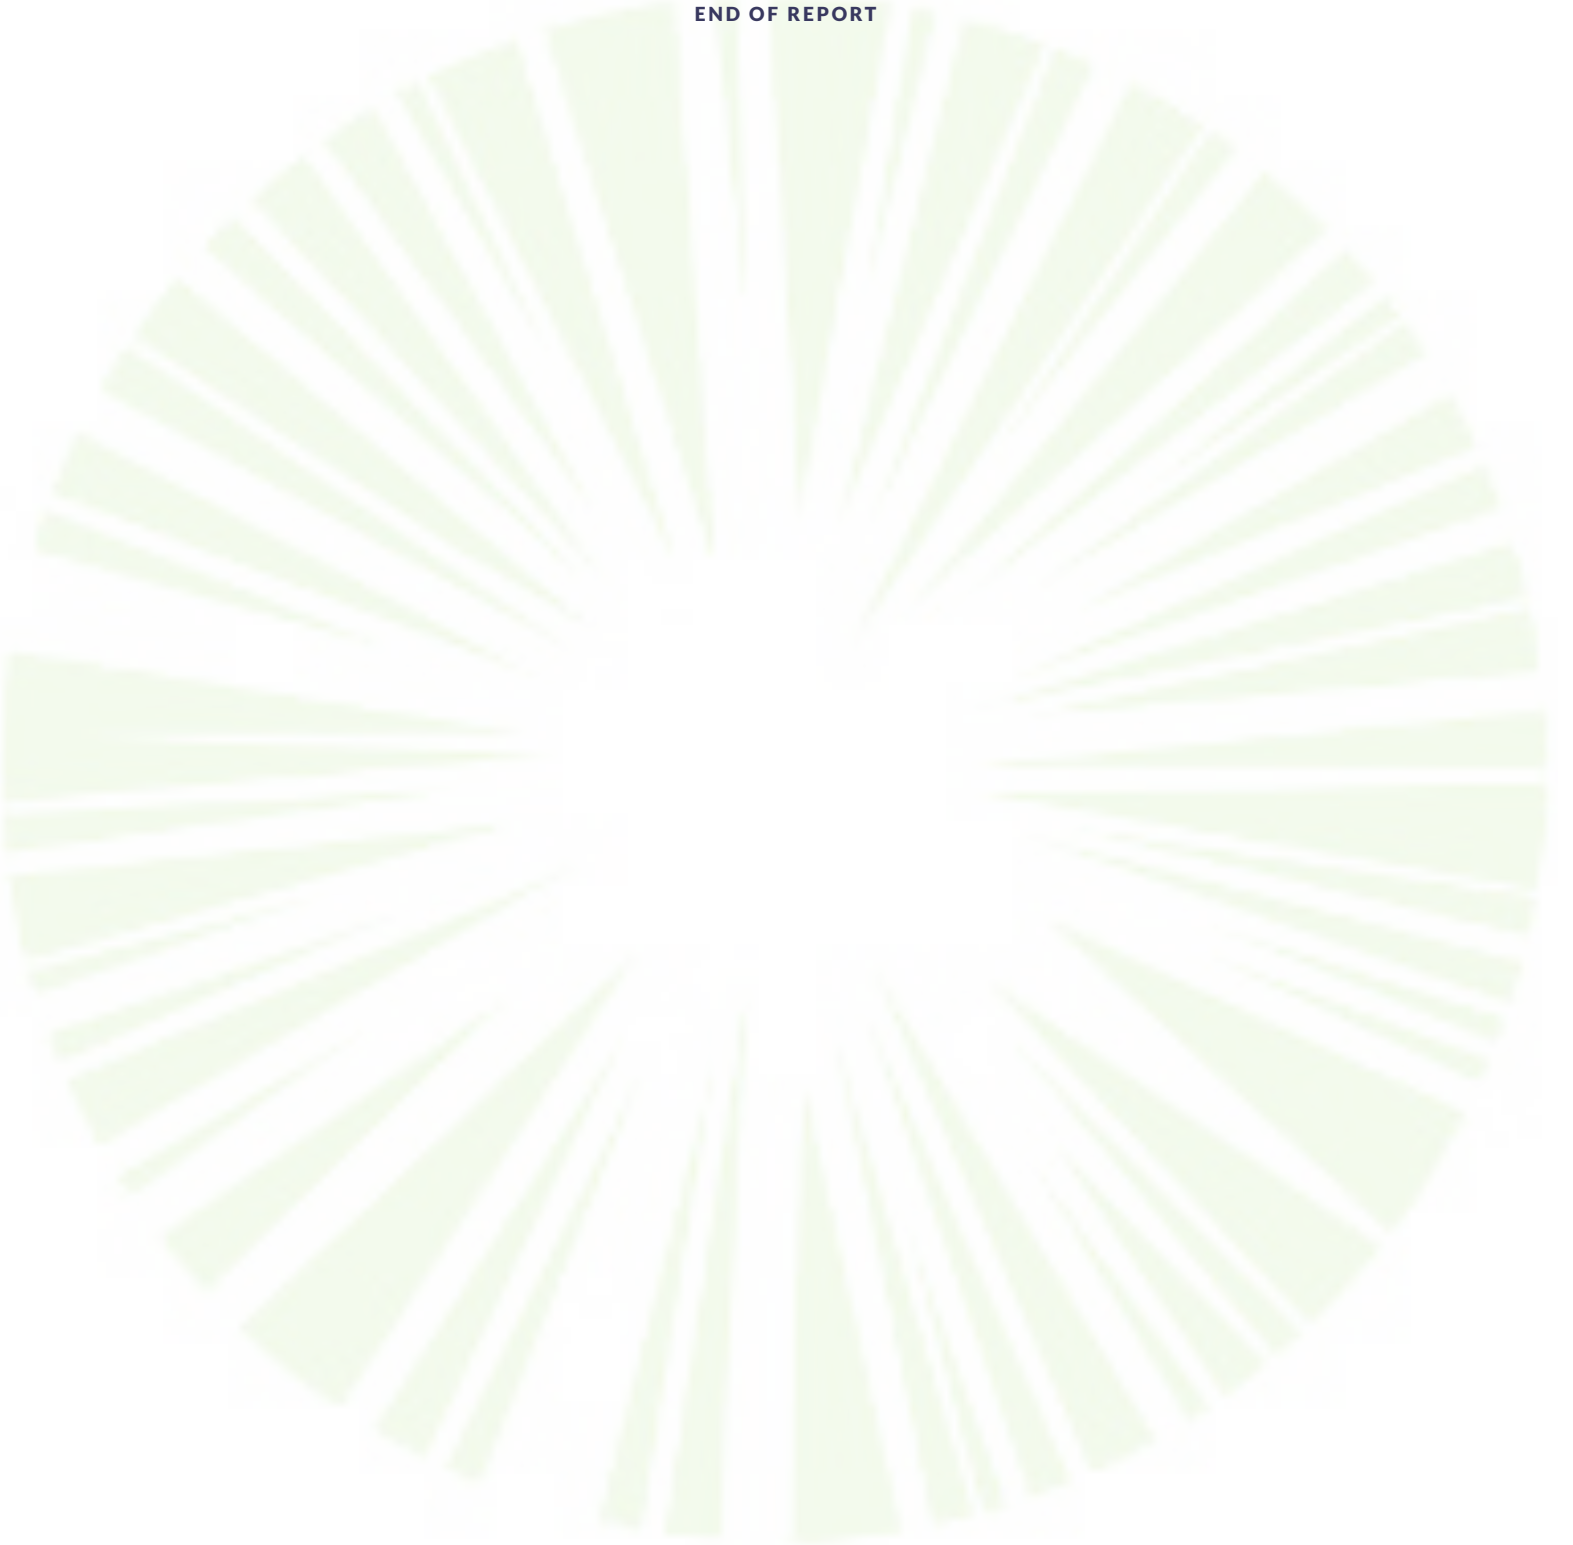


CERTIFICATE OF ANALYSIS

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

CBG.T.23.002-MYCO (TINCTURE) // PRODUCED: AUG 16, 2023

CLIENT: HEALER HEMP LLC // BATCH: PASSED



BATCH NO.: CBG.T.23.002 ¹
MATRIX: TINCTURE ¹
SAMPLE ID: NAL-230808-036
COLLECTED ON: AUG 08, 2023
RECEIVED ON: AUG 08, 2023
SAMPLE SIZE: 2.689 G ¹
SAMPLED BY: ANNA KUPEL
RECEIVED BY: DAGMAR LEMANS

¹ ENTERED BY CLIENT



NOVA ANALYTIC LABS
Tomorrow's Testing, Today.

MANUFACTURER INFO

MANUFACTURER
HEALER HEMP LLC
119 ORION ST
BRUNSWICK, MAINE 04011

LICENSE
CGR26424
MEDICINAL - CAREGIVER

BATCH RESULT: PASSED

MYCOTOXINS TESTED

MYC.1: MYCOTOXINS BY LC-HRMS PREPARATION: AUG 10, 2023 // ANALYSIS: AUG 15, 2023

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
AFLATOXIN B1		ND	0.226/0.677	N/A
AFLATOXIN B2		ND	0.677/1.13	N/A
AFLATOXIN G1		ND	0.226/0.677	N/A

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
AFLATOXIN G2		ND	0.226/1.13	N/A
OCHRATOXIN A		ND	0.451/1.35	N/A



AUTHORIZED BY:

ZACHARY SMITH
LABORATORY MANAGER, NOVA
ANALYTIC LABS
AUG 16, 2023

https://lims.tagleaf.com/coa_/dDsaDg7m02

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OCP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED. THIS CERTIFICATE OF ANALYSIS IS RELEVANT ONLY TO THOSE ITEMS TESTED. THE SAMPLE WAS PROVIDED TO THE LABORATORY FOR TESTING BY THE CLIENT AND THE SAMPLE WAS TESTED AS RECEIVED.


END OF REPORT

CERTIFICATE OF ANALYSIS

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

CBG.T.23.002-MICRO (TINCTURE) // PRODUCED: AUG 11, 2023

CLIENT: HEALER HEMP LLC // BATCH: PASSED



BATCH NO.: CBG.T.23.002 ¹
MATRIX: TINCTURE ¹
SAMPLE ID: NAL-230808-035
COLLECTED ON: AUG 08, 2023
RECEIVED ON: AUG 08, 2023
SAMPLE SIZE: 2.534 G ¹
SAMPLED BY: ANNA KUPEL
RECEIVED BY: DAGMAR LEMANS

¹ ENTERED BY CLIENT



NOVA ANALYTIC LABS
Tomorrow's Testing, Today.

MANUFACTURER INFO

MANUFACTURER
HEALER HEMP LLC
119 ORION ST
BRUNSWICK, MAINE 04011

LICENSE
CGR26424
MEDICINAL - CAREGIVER

BATCH RESULT: PASSED

MICROBIAL TESTED



AUTHORIZED BY:
CHRIS ALTOMARE
CEO, NOVA ANALYTIC LABS
AUG 11, 2023

https://lims.tagleaf.com/coa_/FIVjAySxNZ

MIC.3: TOTAL COLIFORM BY MOST PROBABLE NUMBER
PREPARATION: AUG 08, 2023 // ANALYSIS: AUG 09, 2023

ANALYTE	LIMIT	AMT (CFU/g)	LOD/LOQ (CFU/g)	PASS/FAIL
COLIFORMS	1000 CFU/g	ND	100/100	N/A

MIC.6: TOTAL ENTEROBACTER BY MOST PROBABLE NUMBER
PREPARATION: AUG 08, 2023 // ANALYSIS: AUG 09, 2023

ANALYTE	LIMIT	AMT (CFU/g)	LOD/LOQ (CFU/g)	PASS/FAIL
ENTEROBACTERIACEAE	1000 CFU/g	ND	100/100	N/A

TOTAL AEROBIC BACTERIA BY MOST PROBABLE NUMBER
PREPARATION: AUG 08, 2023 // ANALYSIS: AUG 09, 2023

ANALYTE	LIMIT	AMT (CFU/g)	LOD/LOQ (CFU/g)	PASS/FAIL
AEROBIC BACTERIA	100000 CFU/g	ND	100/100	N/A

MIC.5: SALMONELLA BY PCR
PREPARATION: AUG 08, 2023 // ANALYSIS: AUG 10, 2023

ANALYTE	LIMIT	AMT (CFU/g)	LOD/LOQ (CFU/g)	PASS/FAIL
SALMONELLA SPP.	Any amt in 1 gram	ND	1.00/1.00	N/A

MIC.4: PATHOGENIC E. COLI BY PCR
PREPARATION: AUG 08, 2023 // ANALYSIS: AUG 10, 2023

ANALYTE	LIMIT	AMT (CFU/g)	LOD/LOQ (CFU/g)	PASS/FAIL
SHIGA TOXIN-PRODUCING E. COLI	Any amt in 1 gram	ND	1.00/1.00	N/A

TOTAL YEAST AND MOLD BY MOST PROBABLE NUMBER
PREPARATION: AUG 08, 2023 // ANALYSIS: AUG 11, 2023

ANALYTE	LIMIT	AMT (CFU/g)	LOD/LOQ (CFU/g)	PASS/FAIL
YEAST & MOLD	10000 CFU/g	ND	100/100	N/A

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OCP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED. THIS CERTIFICATE OF ANALYSIS IS RELEVANT ONLY TO THOSE ITEMS TESTED. THE SAMPLE WAS PROVIDED TO THE LABORATORY FOR TESTING BY THE CLIENT AND THE SAMPLE WAS TESTED AS RECEIVED.

END OF REPORT



CERTIFICATE OF ANALYSIS

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

CBG.T.23.002-TERPS (TINCTURE) // PRODUCED: AUG 14, 2023

CLIENT: HEALER HEMP LLC // BATCH: PASSED



BATCH NO.: CBG.T.23.002 ¹
MATRIX: TINCTURE ¹
DENSITY: 0.9236 g/ml ²
SAMPLE ID: NAL-230808-037
COLLECTED ON: AUG 08, 2023
RECEIVED ON: AUG 08, 2023
SAMPLE SIZE: 2.500 G ¹
SAMPLED BY: ANNA KUPEL
RECEIVED BY: DAGMAR LEMANS



NOVA ANALYTIC LABS
 Tomorrow's Testing, Today.

¹ ENTERED BY CLIENT, ² ENTERED BY LAB

MANUFACTURER INFO

MANUFACTURER
 HEALER HEMP LLC
 119 ORION ST
 BRUNSWICK, MAINE 04011

LICENSE
 CGR26424
 MEDICINAL - CAREGIVER

BATCH RESULT: PASSED

TERPENES TESTED

TRP.2: TERPENES BY LIQUID INJECT GCMS PREPARATION: AUG 09, 2023 // ANALYSIS: AUG 10, 2023

ANALYTE	AMT	AMT	LOD/LOQ (mg/ml)	PASS/FAIL
TOTAL TERPENES	0.300 %	2.77 mg/ml		N/A
NEROL	ND	ND	0.156/0.312	N/A
CEDROL	ND	ND	0.156/0.312	N/A
CITRAL	ND	ND	0.156/0.312	N/A
GUAJOL	0.0498 %	0.460 mg/ml	0.156/0.312	N/A
THYMOL	ND	ND	0.156/0.312	N/A
BORNEOL	ND	ND	0.156/0.312	N/A
CAMPHOR	ND	ND	0.156/0.312	N/A
MENTHOL	ND	ND	0.156/0.312	N/A
PHYTANE	ND	ND	0.156/0.312	N/A
CAMPHERE	ND	ND	0.156/0.312	N/A
FARNESOL	ND	ND	0.156/0.312	N/A
FENCHONE	ND	ND	0.156/0.312	N/A
GERANIOL	ND	ND	0.156/0.312	N/A
LINALOOL	ND	ND	0.156/0.312	N/A
MENTHONE	ND	ND	0.156/0.312	N/A
PULEGONE	ND	ND	0.156/0.312	N/A
SABINENE	ND	ND	0.156/0.312	N/A
SAFRANAL	ND	ND	0.156/0.312	N/A
M-CYMENE	ND	ND	0.156/0.312	N/A
O-CYMENE	ND	ND	0.156/0.312	N/A
P-CYMENE	ND	ND	0.156/0.312	N/A
CARVACROL	ND	ND	0.156/0.312	N/A
FARNESENE	ND	ND	0.156/0.312	N/A
TERPINEOL	ND	ND	0.156/0.312	N/A
VALENCENE	ND	ND	0.156/0.312	N/A
D-CARVONE	ND	ND	0.156/0.312	N/A
EUCALYPTOL	ND	ND	0.156/0.312	N/A
ISOBORNEOL	ND	ND	0.156/0.312	N/A
ISOPULEGOL	ND	ND	0.156/0.312	N/A

ANALYTE	AMT	AMT	LOD/LOQ (mg/ml)	PASS/FAIL
PIPERITONE	ND	ND	0.156/0.312	N/A
D-LIMONENE	ND	ND	0.156/0.312	N/A
CITRONELLOL	ND	ND	0.156/0.312	N/A
E-NEROLIDOL	ND	ND	0.156/0.312	N/A
TERPINOLENE	ND	ND	0.156/0.312	N/A
Z-NEROLIDOL	ND	ND	0.156/0.312	N/A
β-PINENE	ND	ND	0.156/0.312	N/A
2-PIPERIDONE	ND	ND	0.156/0.312	N/A
α-PINENE	ND	ND	0.156/0.312	N/A
β-MYRCENE	ND	ND	0.156/0.312	N/A
(-)-VERBENONE	ND	ND	0.156/0.312	N/A
OCTYL ACETATE	ND	ND	0.156/0.312	N/A
TERPINEN-4-OL	ND	ND	0.156/0.312	N/A
α-CEDRENE	ND	ND	0.156/0.312	N/A
α-THUJONE	ND	ND	0.156/0.312	N/A
Δ³-CARENE	ND	ND	0.156/0.312	N/A
α-HUMULENE	0.0440 %	0.406 mg/ml	0.156/0.312	N/A
GERANYL ACETATE	ND	ND	0.156/0.312	N/A
α-BISABOLOL	0.0848 %	0.783 mg/ml	0.156/0.312	N/A
α-TERPINENE	ND	ND	0.156/0.312	N/A
γ-TERPINENE	ND	ND	0.156/0.312	N/A
SABINENE HYDRATE	ND	ND	0.156/0.312	N/A
CIS-β-OCIMENE	ND	ND	0.156/0.312	N/A
ISOBORNYL ACETATE	ND	ND	0.156/0.312	N/A
α-PHELLANDRENE	ND	ND	0.156/0.312	N/A
β-CARYOPHYLLENE	0.121 %	1.12 mg/ml	0.156/0.312	N/A
TRANS-β-OCIMENE	ND	ND	0.156/0.312	N/A
CARYOPHYLLENE OXIDE	ND	ND	0.156/0.312	N/A
ENDO FENCHYL ALCOHOL	ND	ND	0.156/0.312	N/A



https://lims.tagleaf.com/coa_/wc7ZqeUmfX

** FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.*

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OCP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED. THIS CERTIFICATE OF ANALYSIS IS RELEVANT ONLY TO THOSE ITEMS TESTED. THE SAMPLE WAS PROVIDED TO THE LABORATORY FOR TESTING BY THE CLIENT AND THE SAMPLE WAS TESTED AS RECEIVED.

END OF REPORT




CERTIFICATE OF ANALYSIS

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

CBG.T.23.002-SOLV (TINCTURE) // PRODUCED: AUG 10, 2023

CLIENT: HEALER HEMP LLC // BATCH: PASSED



BATCH NO.: CBG.T.23.002 ¹
MATRIX: TINCTURE ¹
SAMPLE ID: NAL-230808-038
COLLECTED ON: AUG 08, 2023
RECEIVED ON: AUG 08, 2023
SAMPLE SIZE: 2.729 G ¹
SAMPLED BY: ANNA KUPPEL
RECEIVED BY: DAGMAR LEMANS

¹ ENTERED BY CLIENT



NOVA ANALYTIC LABS
 Tomorrow's Testing, Today.

MANUFACTURER INFO

MANUFACTURER
 HEALER HEMP LLC
 119 ORION ST
 BRUNSWICK, MAINE 04011
LICENSE
 CGR26424
 MEDICINAL - CAREGIVER

BATCH RESULT: PASSED

SOLVENTS TESTED

RSOL.1: RESIDUAL SOLVENTS, POISONS AND TOXINS BY HEADSPACE GC-MS PREPARATION: AUG 09, 2023 // ANALYSIS: AUG 09, 2023

ANALYTE	LIMIT	AMT (µg/g)	LOD/LOQ (µg/g)	PASS/FAIL
BUTANE	5000 µg/g	ND	0.941/2.35	N/A
HEXANE	290 µg/g	ND	0.941/2.35	N/A
ACETONE	5000 µg/g	ND	47.1/94.1	N/A
BENZENE	1 µg/g	ND	0.471/0.941	N/A
ETHANOL	5000 µg/g	8190	18.8/47.1	N/A
HEPTANE	5000 µg/g	ND	9.41/18.8	N/A
PENTANE	5000 µg/g	ND	9.41/18.8	N/A
PROPANE	5000 µg/g	ND	18.8/37.6	N/A
TOLUENE	890 µg/g	ND	4.71/9.41	N/A
METHANOL	3000 µg/g	ND	47.1/94.1	N/A
O-XYLENE	2170 µg/g	ND	9.41/18.8	N/A

ANALYTE	LIMIT	AMT (µg/g)	LOD/LOQ (µg/g)	PASS/FAIL
CHLOROFORM	1 µg/g	ND	0.471/0.941	N/A
ETHYL ETHER	5000 µg/g	ND	9.41/18.8	N/A
ACETONITRILE	410 µg/g	ND	9.41/18.8	N/A
ETHYL ACETATE	5000 µg/g	ND	9.41/18.8	N/A
ETHYLENE OXIDE	1 µg/g	ND	0.471/0.941	N/A
P- AND M-XYLENE	2170 µg/g	ND	18.8/37.6	N/A
ISOPROPYL ALCOHOL	5000 µg/g	ND	47.1/94.1	N/A
TRICHLOROETHYLENE	1 µg/g	ND	0.471/0.941	N/A
1,2-DICHLOROETHANE	1 µg/g	ND	0.471/0.941	N/A
METHYLENE CHLORIDE	1 µg/g	ND	0.471/0.941	N/A



AUTHORIZED BY:
 GREG NEWLAND
 CSO, NOVA ANALYTIC LABS
 AUG 10, 2023



https://lims.tagleaf.com/coa_vhmabAU8R3


* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OCP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED. THIS CERTIFICATE OF ANALYSIS IS RELEVANT ONLY TO THOSE ITEMS TESTED. THE SAMPLE WAS PROVIDED TO THE LABORATORY FOR TESTING BY THE CLIENT AND THE SAMPLE WAS TESTED AS RECEIVED.

END OF REPORT

CERTIFICATE OF ANALYSIS

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

H.21-001 MT (EXTRACT) // PRODUCED: MAY 10, 2021**CLIENT: HEALER HEMP LLC // BATCH: PASSED AS MAINE INDUSTRIAL HEMP**

BATCH NO.: H.21-001
MATRIX: EXTRACT
SAMPLE ID: NAL-210507-007
COLLECTED ON: MAY 07, 2021
RECEIVED ON: MAY 07, 2021
SAMPLE SIZE: 5.452 GRAMS
RECEIVED BY: ANDREW PATTERSON

**NOVA ANALYTIC LABS**
Tomorrow's Testing, Today.**MANUFACTURER INFO**

MANUFACTURER
HEALER HEMP LLC
119 ORION ST
BRUNSWICK, MAINE 04011

LICENSE
CGR26424
MEDICINAL - CAREGIVER

BATCH RESULT: PASSED AS MAINE INDUSTRIAL HEMP**METALS** TESTED**HME.1: HEAVY METALS BY ICP-MS**
PREPARATION: MAY 10, 2021 // ANALYSIS: MAY 10, 2021

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
LEAD	500 µg/kg	ND	20.1/60.2	N/A
ARSENIC	200 µg/kg	< LOQ	20.1/50.1	N/A

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
CADMIUM	200 µg/kg	ND	20.1/50.1	N/A
MERCURY	100 µg/kg	ND	20.1/40.1	N/A



RESULTS CERTIFIED BY:
BARRY CHAFFIN
COO, NOVA ANALYTIC LABS
MAY 10, 2021

RESULTS CERTIFIED BY:
GREG NEWLAND
CSO, NOVA ANALYTIC LABS
MAY 10, 2021

RESULTS CERTIFIED BY:
CHRIS ALTOMARE
CEO, NOVA ANALYTIC LABS
MAY 10, 2021

https://lims.tagleaf.com/coa_/ZDgj5hE2d1

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OMP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED.

END OF REPORT




CERTIFICATE OF ANALYSIS

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

H.21-001 PESTICIDE TEST (TINCTURE) // PRODUCED: JUL 06, 2021

CLIENT: HEALER HEMP LLC // BATCH: PASSED AS MAINE INDUSTRIAL HEMP



BATCH NO.: H.21-001
MATRIX: TINCTURE
SAMPLE ID: NAL-210702-015
COLLECTED ON: JUL 02, 2021
RECEIVED ON: JUL 02, 2021
SAMPLE SIZE: 3.936 G



NOVA ANALYTIC LABS
Tomorrow's Testing, Today.

MANUFACTURER INFO

MANUFACTURER
HEALER HEMP LLC
119 ORION ST
BRUNSWICK, MAINE 04011

LICENSE
CGR26424
MEDICINAL - CAREGIVER

BATCH RESULT: PASSED AS MAINE INDUSTRIAL HEMP

PESTICIDES TESTED

PES.1: PESTICIDES, INSECTICIDES, FUNGICIDES AND GROWTH REGULATORS BY LC-MS/MS
PREPARATION: JUL 02, 2021 // ANALYSIS: JUL 02, 2021

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL	ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
IMAZALIL		ND	2.86/5.72	N/A	DAMINOZIDE		ND	28.6/28.6	N/A
ETOXAZOLE		ND	2.86/5.72	N/A	MYCLOBUTANIL		ND	1.43/5.72	N/A
BIFENTHRIN		ND	2.86/5.72	N/A	SPIROMESIFEN		ND	2.86/5.72	N/A
CYFLUTHRIN		ND	28.6/28.6	N/A	TRIFLOXYSTROB-IN		ND	1.43/5.72	N/A



RESULTS CERTIFIED BY:
BARRY CHAFFIN
COO, NOVA ANALYTIC LABS
JUL 06, 2021

RESULTS CERTIFIED BY:
GREG NEWLAND
CSO, NOVA ANALYTIC LABS
JUL 06, 2021

RESULTS CERTIFIED BY:
CHRIS ALTOMARE
CEO, NOVA ANALYTIC LABS
JUL 06, 2021

https://lims.tagleaf.com/coa_sVTqDHmMyf

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OMP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED.


END OF REPORT

CERTIFICATE OF ANALYSIS

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

H.22.004.D-BCT-PEST (TINCTURE) // PRODUCED: OCT 03, 2022

CLIENT: HEALER HEMP LLC // BATCH: PASSED



BATCH NO.: H.22.004.D-BCT
MATRIX: TINCTURE
SAMPLE ID: NAL-220929-002
COLLECTED ON: SEP 29, 2022
RECEIVED ON: SEP 29, 2022
SAMPLE SIZE: 1.174 G
SAMPLED BY: ANNA KUPEL
RECEIVED BY: KENDALL ERICKSEN



NOVA ANALYTIC LABS
Tomorrow's Testing, Today.

MANUFACTURER INFO

MANUFACTURER
HEALER HEMP LLC
119 ORION ST
BRUNSWICK, MAINE 04011

LICENSE
CGR26424
MEDICINAL - CAREGIVER

BATCH RESULT: PASSED

PESTICIDES TESTED

PST.2: PESTICIDES, INSECTICIDES, FUNGICIDES AND GROWTH REGULATORS BY LC-HRMS
PREPARATION: OCT 01, 2022 // ANALYSIS: OCT 03, 2022

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL	ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
NALED	500 µg/kg	ND	125/125	N/A	METHIOCARB	200 µg/kg	ND	125/125	N/A
OXAMYL	1000 µg/kg	ND	125/125	N/A	ACEQUINOCYL	2000 µg/kg	ND	125/125	N/A
PHOSMET	200 µg/kg	ND	125/125	N/A	ACETAMIPRID	200 µg/kg	ND	125/125	N/A
ACEPHATE	400 µg/kg	ND	125/125	N/A	ETHOPROPHOS	200 µg/kg	ND	125/125	N/A
ALDICARB	400 µg/kg	ND	125/125	N/A	FLUDIOXONIL	400 µg/kg	ND	125/125	N/A
BOSCALID	400 µg/kg	ND	125/125	N/A	HEXYTHIAZOX	1000 µg/kg	ND	125/125	N/A
CARBARYL	200 µg/kg	ND	125/125	N/A	PRALLETHRIN	200 µg/kg	ND	125/125	N/A
DIAZINON	200 µg/kg	ND	125/125	N/A	SPIROXAMINE	400 µg/kg	ND	125/125	N/A
FIPRONIL	400 µg/kg	ND	125/125	N/A	THIACLOPRID	200 µg/kg	ND	125/125	N/A
IMAZALIL	200 µg/kg	ND	125/125	N/A	AZOXYSTROBIN	200 µg/kg	ND	125/125	N/A
METHOMYL	400 µg/kg	ND	125/125	N/A	CHLORFENAPYR	1000 µg/kg	ND	125/167	N/A
PROPOXUR	200 µg/kg	ND	125/125	N/A	CHLORPYRIFOS	200 µg/kg	ND	125/125	N/A
SPINOSAD	200 µg/kg	ND	125/125	N/A	CLOFENTEZINE	200 µg/kg	ND	125/125	N/A
ABAMECTIN	500 µg/kg	ND	125/125	N/A	CYPERMETHRIN	1000 µg/kg	ND	417/835	N/A
ETOXAZOLE	200 µg/kg	ND	125/125	N/A	IMIDACLOPRID	400 µg/kg	ND	125/125	N/A
MGK-264 I		ND	125/125	N/A	MYCLOBUTANIL	200 µg/kg	ND	125/125	N/A
MALATHION	200 µg/kg	ND	125/125	N/A	SPIROMESIFEN	200 µg/kg	ND	125/125	N/A
METALAXYL	200 µg/kg	ND	125/125	N/A	TEBUCONAZOLE	400 µg/kg	ND	125/125	N/A
PYRIDABEN	200 µg/kg	ND	125/125	N/A	THIAMETHOXAM	200 µg/kg	ND	125/125	N/A
BIFENAZATE	200 µg/kg	ND	125/125	N/A	FENPYROXIMATE	400 µg/kg	ND	125/125	N/A
BIFENTHRIN	200 µg/kg	ND	125/125	N/A	PACLOBUTRAZOL	400 µg/kg	ND	125/125	N/A
CARBOFURAN	200 µg/kg	ND	125/125	N/A	PROPICONAZOLE	400 µg/kg	ND	167/167	N/A
CYFLUTHRIN	1000 µg/kg	ND	417/835	N/A	SPIROTETRAMAT	200 µg/kg	ND	125/125	N/A
DAMINOZIDE	1000 µg/kg	ND	417/835	N/A	PERMETHRIN CIS		ND	125/125	N/A
DICHLORVOS	1000 µg/kg	ND	125/125	N/A	KRESOXIM-METHYL	400 µg/kg	ND	125/125	N/A
DIMETHOATE	200 µg/kg	ND	125/125	N/A	TRIFLOXYSTROBIN	200 µg/kg	ND	125/125	N/A
ETOXENPROX	200 µg/kg	ND	125/125	N/A	PARATHION-METHYL	200 µg/kg	ND	125/125	N/A
FENOXYCARB	200 µg/kg	ND	125/125	N/A	PERMETHRIN TRANS		ND	125/125	N/A
FLONICAMID	1000 µg/kg	ND	125/125	N/A	PIPERONYLBUTOXIDE	2000 µg/kg	ND	125/125	N/A
MGK-264 II		ND	125/125	N/A					



RESULTS CERTIFIED BY:
BARRY CHAFFIN
COO, NOVA ANALYTIC LABS
OCT 03, 2022

RESULTS CERTIFIED BY:
GREG NEWLAND
CSO, NOVA ANALYTIC LABS
OCT 03, 2022

RESULTS CERTIFIED BY:
CHRIS ALTOMARE
CEO, NOVA ANALYTIC LABS
OCT 03, 2022

https://lims.tagleaf.com/coa_/x8tvbanCgu

NOTES

CHRIS ALTOMARE
OCT 03, 2022

PESTICIDES, INSECTICIDES, FUNGICIDES AND GROWTH REGULATORS BY LC-HRMS
ANALYSIS FOR NALED AND CLOFENTEZINE ARE QUALITATIVE ONLY. ANY NUMBER INDICATES DETECTION AND ACTUAL CONCENTRATION SHOULD NOT BE INTERPRETED QUANTITATIVELY.

** FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.*

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OMP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED.

END OF REPORT




CERTIFICATE OF ANALYSIS

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

H.22.004.D-BCT-METALS (TINCTURE) // PRODUCED: OCT 04, 2022

CLIENT: HEALER HEMP LLC // BATCH: PASSED



BATCH NO.: H.22.004.D-BCT
MATRIX: TINCTURE
SAMPLE ID: NAL-220929-003
COLLECTED ON: SEP 29, 2022
RECEIVED ON: SEP 29, 2022
SAMPLE SIZE: 1.718 G
SAMPLED BY: ANNA KUPEL
RECEIVED BY: KENDALL ERICKSEN



NOVA ANALYTIC LABS
Tomorrow's Testing, Today.

MANUFACTURER INFO

MANUFACTURER
HEALER HEMP LLC
119 ORION ST
BRUNSWICK, MAINE 04011

LICENSE
CGR26424
MEDICINAL - CAREGIVER

BATCH RESULT: PASSED

METALS TESTED

HME.1: HEAVY METALS BY ICP-MS PREPARATION: OCT 04, 2022 // ANALYSIS: OCT 04, 2022

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
LEAD	500 µg/kg	ND	34.8/104	N/A
ARSENIC	1500 µg/kg	ND	34.8/86.9	N/A

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
CADMIUM	500 µg/kg	ND	34.8/86.9	N/A
MERCURY	3000 µg/kg	ND	34.8/69.5	N/A



RESULTS CERTIFIED BY:
BARRY CHAFFIN
COO, NOVA ANALYTIC LABS
OCT 04, 2022

RESULTS CERTIFIED BY:
GREG NEWLAND
CSO, NOVA ANALYTIC LABS
OCT 04, 2022

RESULTS CERTIFIED BY:
CHRIS ALTOMARE
CEO, NOVA ANALYTIC LABS
OCT 04, 2022

https://lims.tagleaf.com/coa/_YXYr6TNrNr

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OMP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED.


END OF REPORT

CERTIFICATE OF ANALYSIS

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

H.22.005.A-PEST (TINCTURE) // PRODUCED: NOV 08, 2022

CLIENT: HEALER HEMP LLC // BATCH: PASSED



BATCH NO.: H.22.005.A-BCT
MATRIX: TINCTURE
SAMPLE ID: NAL-221107-004
COLLECTED ON: NOV 07, 2022
RECEIVED ON: NOV 07, 2022
SAMPLE SIZE: 3.050 G
SAMPLED BY: ANNA KUPEL
RECEIVED BY: NICHOLAS CHAMBERLAIN



NOVA ANALYTIC LABS
Tomorrow's Testing, Today.

MANUFACTURER INFO

MANUFACTURER
HEALER HEMP LLC
119 ORION ST
BRUNSWICK, MAINE 04011

LICENSE
CGR26424
MEDICINAL - CAREGIVER

BATCH RESULT: PASSED

PESTICIDES TESTED

PST.2: PESTICIDES, INSECTICIDES, FUNGICIDES AND GROWTH REGULATORS BY LC-HRMS
PREPARATION: NOV 07, 2022 // ANALYSIS: NOV 07, 2022

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL	ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
NALED	500 µg/kg	ND	130/130	N/A	METHIOCARB	200 µg/kg	ND	130/130	N/A
OXAMYL	1000 µg/kg	ND	130/130	N/A	ACEQUINOCYL	2000 µg/kg	ND	130/130	N/A
PHOSMET	200 µg/kg	ND	130/130	N/A	ACETAMIPRID	200 µg/kg	ND	130/130	N/A
ACEPHATE	400 µg/kg	ND	130/130	N/A	ETHOPROPHOS	200 µg/kg	ND	130/130	N/A
ALDICARB	400 µg/kg	ND	130/130	N/A	FLUDIOXONIL	400 µg/kg	ND	130/130	N/A
BOSCALID	400 µg/kg	ND	130/130	N/A	HEXYTHIAZOX	1000 µg/kg	ND	130/130	N/A
CARBARYL	200 µg/kg	ND	130/130	N/A	PRALLETHRIN	200 µg/kg	ND	130/130	N/A
DIAZINON	200 µg/kg	ND	130/130	N/A	SPIROXAMINE	400 µg/kg	ND	130/130	N/A
FIPRONIL	400 µg/kg	ND	130/130	N/A	THIACLOPRID	200 µg/kg	ND	130/130	N/A
IMAZALIL	200 µg/kg	ND	130/130	N/A	AZOXYSTROBIN	200 µg/kg	ND	130/130	N/A
METHOMYL	400 µg/kg	ND	130/130	N/A	CHLORFENAPYR	1000 µg/kg	ND	130/173	N/A
PROPOXUR	200 µg/kg	ND	130/130	N/A	CHLORPYRIFOS	200 µg/kg	ND	130/130	N/A
SPINOSAD	200 µg/kg	ND	130/130	N/A	CLOFENTEZINE	200 µg/kg	ND	130/130	N/A
ABAMECTIN	500 µg/kg	ND	130/130	N/A	CYPERMETHRIN	1000 µg/kg	ND	434/867	N/A
ETOXAZOLE	200 µg/kg	ND	130/130	N/A	IMIDACLOPRID	400 µg/kg	ND	130/130	N/A
MGK-264 I		ND	130/130	N/A	MYCLOBUTANIL	200 µg/kg	ND	130/130	N/A
MALATHION	200 µg/kg	ND	130/130	N/A	SPIROMESIFEN	200 µg/kg	ND	130/130	N/A
METALAXYL	200 µg/kg	ND	130/130	N/A	TEBUCONAZOLE	400 µg/kg	ND	130/130	N/A
PYRIDABEN	200 µg/kg	ND	130/130	N/A	THIAMETHOXAM	200 µg/kg	ND	130/130	N/A
BIFENAZATE	200 µg/kg	ND	130/130	N/A	FENPYROXIMATE	400 µg/kg	ND	130/130	N/A
BIFENTHRIN	200 µg/kg	ND	130/130	N/A	PACLOBUTRAZOL	400 µg/kg	ND	130/130	N/A
CARBOFURAN	200 µg/kg	ND	130/130	N/A	PROPICONAZOLE	400 µg/kg	ND	173/173	N/A
CYFLUTHRIN	1000 µg/kg	ND	434/867	N/A	SPIROTETRAMAT	200 µg/kg	ND	130/130	N/A
DAMINOZIDE	1000 µg/kg	ND	434/867	N/A	PERMETHRIN CIS		ND	130/130	N/A
DICHLORVOS	1000 µg/kg	ND	130/130	N/A	KRESOXIM-METHYL	400 µg/kg	ND	130/130	N/A
DIMETHOATE	200 µg/kg	ND	130/130	N/A	TRIFLOXYSTROB-IN	200 µg/kg	ND	130/130	N/A
ETOXENPROX	200 µg/kg	ND	130/130	N/A	PARATHION-METHYL	200 µg/kg	ND	130/130	N/A
FENOXYCARB	200 µg/kg	ND	130/130	N/A	PERMETHRIN TRANS		ND	130/130	N/A
FLONICAMID	1000 µg/kg	ND	130/130	N/A	PIPERONYLBUTO-XIDE	2000 µg/kg	ND	130/130	N/A
MGK-264 II		ND	130/130	N/A					



RESULTS CERTIFIED BY:
BARRY CHAFFIN
COO, NOVA ANALYTIC LABS
NOV 08, 2022

RESULTS CERTIFIED BY:
GREG NEWLAND
CSO, NOVA ANALYTIC LABS
NOV 08, 2022

RESULTS CERTIFIED BY:
CHRIS ALTOMARE
CEO, NOVA ANALYTIC LABS
NOV 08, 2022

https://lims.tagleaf.com/coa_/ICL7B54iJ6

NOTES

CHRIS ALTOMARE
NOV 08, 2022

PESTICIDES, INSECTICIDES, FUNGICIDES AND GROWTH REGULATORS BY LC-HRMS
ANALYSIS FOR NALED AND CLOFENTEZINE ARE QUALITATIVE ONLY. ANY NUMBER INDICATES DETECTION AND ACTUAL CONCENTRATION SHOULD NOT BE INTERPRETED QUANTITATIVELY.

** FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.*

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OMP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED.

END OF REPORT




CERTIFICATE OF ANALYSIS

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

H.22.005.A-METALS (TINCTURE) // PRODUCED: NOV 10, 2022

CLIENT: HEALER HEMP LLC // BATCH: PASSED



BATCH NO.: H.22.005.A-BCT
MATRIX: TINCTURE
SAMPLE ID: NAL-221107-003
COLLECTED ON: NOV 07, 2022
RECEIVED ON: NOV 07, 2022
SAMPLE SIZE: 2.418 G
SAMPLED BY: ANNA KUPEL
RECEIVED BY: NICHOLAS CHAMBERLAIN



NOVA ANALYTIC LABS
Tomorrow's Testing, Today.

MANUFACTURER INFO

MANUFACTURER
HEALER HEMP LLC
119 ORION ST
BRUNSWICK, MAINE 04011

LICENSE
CGR26424
MEDICINAL - CAREGIVER

BATCH RESULT: PASSED

METALS TESTED

HME.1: HEAVY METALS BY ICP-MS PREPARATION: NOV 09, 2022 // ANALYSIS: NOV 09, 2022

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
LEAD	500 µg/kg	ND	34.7/104	N/A
ARSENIC	1500 µg/kg	ND	34.7/86.7	N/A

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
CADMIUM	500 µg/kg	ND	34.7/86.7	N/A
MERCURY	3000 µg/kg	ND	34.7/69.4	N/A



RESULTS CERTIFIED BY:
BARRY CHAFFIN
COO, NOVA ANALYTIC LABS
NOV 10, 2022

RESULTS CERTIFIED BY:
GREG NEWLAND
CSO, NOVA ANALYTIC LABS
NOV 10, 2022

RESULTS CERTIFIED BY:
CHRIS ALTOMARE
CEO, NOVA ANALYTIC LABS
NOV 10, 2022

https://lims.tagleaf.com/coa_/DzZcXbHOZr

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OMP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED.

END OF REPORT

CERTIFICATE OF ANALYSIS

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

H.22.007-METALS (TINCTURE) // PRODUCED: DEC 22, 2022

CLIENT: HEALER HEMP LLC // BATCH: PASSED



BATCH NO.: H.22.007
MATRIX: TINCTURE
SAMPLE ID: NAL-221219-003
COLLECTED ON: DEC 19, 2022
RECEIVED ON: DEC 19, 2022
SAMPLE SIZE: 1.961 G
SAMPLED BY: ANNA KUPEL
RECEIVED BY: KAYLIN KEITH



NOVA ANALYTIC LABS
Tomorrow's Testing, Today.

MANUFACTURER INFO

MANUFACTURER
HEALER HEMP LLC
119 ORION ST
BRUNSWICK, MAINE 04011

LICENSE
CGR26424
MEDICINAL - CAREGIVER

BATCH RESULT: PASSED

METALS TESTED

HME.1: HEAVY METALS BY ICP-MS
PREPARATION: DEC 20, 2022 // ANALYSIS: DEC 20, 2022

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
LEAD	500 µg/kg	ND	33.2/99.6	N/A
ARSENIC	1500 µg/kg	ND	33.2/83.0	N/A

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
CADMIUM	500 µg/kg	ND	33.2/83.0	N/A
MERCURY	3000 µg/kg	ND	33.2/66.4	N/A



RESULTS CERTIFIED BY:
BARRY CHAFFIN
COO, NOVA ANALYTIC LABS
DEC 22, 2022

RESULTS CERTIFIED BY:
GREG NEWLAND
CSO, NOVA ANALYTIC LABS
DEC 22, 2022

RESULTS CERTIFIED BY:
CHRIS ALTOMARE
CEO, NOVA ANALYTIC LABS
DEC 22, 2022

https://lims.tagleaf.com/coa/_Y2SRWoUZli

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OMP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED.


END OF REPORT

CERTIFICATE OF ANALYSIS

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

H.22.007-PEST (TINCTURE) // PRODUCED: DEC 21, 2022

CLIENT: HEALER HEMP LLC // BATCH: PASSED



BATCH NO.: H.22.007
MATRIX: TINCTURE
SAMPLE ID: NAL-221219-004
COLLECTED ON: DEC 19, 2022
RECEIVED ON: DEC 19, 2022
SAMPLE SIZE: 1.973 G
SAMPLED BY: ANNA KUPEL
RECEIVED BY: KAYLIN KEITH



NOVA ANALYTIC LABS
 Tomorrow's Testing, Today.

MANUFACTURER INFO

MANUFACTURER
 HEALER HEMP LLC
 119 ORION ST
 BRUNSWICK, MAINE 04011

LICENSE
 CGR26424
 MEDICINAL - CAREGIVER

BATCH RESULT: PASSED

PESTICIDES TESTED

: PESTICIDES, INSECTICIDES, FUNGICIDES AND GROWTH REGULATORS BY LC-HRMS
PREPARATION: DEC 19, 2022 // ANALYSIS: DEC 19, 2022

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
NALED	500 µg/kg	ND	132/177	N/A
OXAMYL	1000 µg/kg	ND	132/441	N/A
PHOSMET	200 µg/kg	ND	132/132	N/A
ACEPHATE	400 µg/kg	ND	132/177	N/A
ALDICARB	400 µg/kg	ND	132/177	N/A
BOSCALID	400 µg/kg	ND	132/177	N/A
CARBARYL	200 µg/kg	ND	132/132	N/A
DIAZINON	200 µg/kg	ND	132/132	N/A
FIPRONIL	400 µg/kg	ND	132/177	N/A
IMAZALIL	200 µg/kg	ND	132/132	N/A
METHOMYL	400 µg/kg	ND	132/177	N/A
PROPOXUR	200 µg/kg	ND	132/132	N/A
SPINOSAD	200 µg/kg	ND	132/132	N/A
ABAMECTIN	500 µg/kg	ND	132/177	N/A
ETOXAZOLE	200 µg/kg	ND	132/132	N/A
MGK-264 I		ND	80.7/80.7	N/A
MALATHION	200 µg/kg	ND	132/132	N/A
METALAXYL	200 µg/kg	ND	132/132	N/A
PYRIDABEN	200 µg/kg	ND	132/132	N/A
BIFENAZATE	200 µg/kg	ND	132/132	N/A
BIFENTHRIN	200 µg/kg	ND	132/132	N/A
CARBOFURAN	200 µg/kg	ND	132/132	N/A
CYFLUTHRIN	1000 µg/kg	ND	132/441	N/A
DAMINOZIDE	1000 µg/kg	ND	132/441	N/A
DICHLORVOS	1000 µg/kg	ND	132/441	N/A
DIMETHOATE	200 µg/kg	ND	132/132	N/A
ETOXENPROX	400 µg/kg	ND	132/177	N/A
FENOXYCARB	200 µg/kg	ND	132/132	N/A
FLONICAMID	1000 µg/kg	ND	132/441	N/A
MGK-264 II		ND	51.6/51.6	N/A
METHIOCARB	200 µg/kg	ND	132/132	N/A
ACEQUINOCYL	2000 µg/kg	ND	132/882	N/A
ACETAMIPRID	200 µg/kg	ND	132/132	N/A

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
ETHOPROPHOS	200 µg/kg	ND	132/132	N/A
FLUDIOXONIL	400 µg/kg	ND	132/177	N/A
HEXYTHIAZOX	1000 µg/kg	ND	132/441	N/A
PRALLETHRIN	200 µg/kg	ND	132/132	N/A
SPIROXAMINE	400 µg/kg	ND	132/177	N/A
THIACLOPRID	200 µg/kg	ND	132/132	N/A
AZOXYSTROBIN	200 µg/kg	ND	132/132	N/A
CHLORFENAPYR	1000 µg/kg	ND	132/441	N/A
CHLORPYRIFOS	200 µg/kg	ND	132/132	N/A
CLOFENTEZINE	200 µg/kg	ND	132/132	N/A
CYPERMETHRIN	1000 µg/kg	ND	132/441	N/A
IMIDACLOPRID	400 µg/kg	ND	132/177	N/A
MYCLOBUTANIL	200 µg/kg	ND	132/132	N/A
SPIROMESIFEN	200 µg/kg	ND	132/132	N/A
TEBUCONAZOLE	400 µg/kg	ND	132/177	N/A
THIAMETHOXAM	200 µg/kg	ND	132/132	N/A
FENPYROXIMATE	400 µg/kg	ND	132/177	N/A
PACLOBUTRAZOL	400 µg/kg	ND	132/177	N/A
PROPICONAZOLE	400 µg/kg	ND	132/177	N/A
SPIROTETRAMAT	200 µg/kg	ND	132/132	N/A
PERMETHRIN CIS		ND	56.9/56.9	N/A
KRESOXIM-METHYL	400 µg/kg	ND	132/177	N/A
TRIFLOXYSTROBIN	200 µg/kg	ND	132/132	N/A
PARATHION-METHYL	200 µg/kg	ND	132/132	N/A
PERMETHRIN TRANS		ND	75.4/75.4	N/A
PIPERONYLBUTOXIDE	2000 µg/kg	ND	132/882	N/A

CHLORANTRANIL-IPROLE	200 µg/kg	ND	132/132	N/A
PYRETHRINS CINERIN I		ND	88.1/88.1	N/A
PYRETHRINS CINERIN II		ND	90.0/90.0	N/A
PYRETHRINS JASMOLIN I		ND	71.5/71.5	N/A
PYRETHRINS JASMOLIN II		ND	55.6/55.6	N/A
PYRETHRINS PYRETHRIN I		ND	410/410	N/A
PYRETHRINS PYRETHRIN II		ND	242/242	N/A



RESULTS CERTIFIED BY:
BARRY CHAFFIN
COO, NOVA ANALYTIC LABS
DEC 21, 2022

RESULTS CERTIFIED BY:
GREG NEWLAND
CSO, NOVA ANALYTIC LABS
DEC 21, 2022

RESULTS CERTIFIED BY:
CHRIS ALTOMARE
CEO, NOVA ANALYTIC LABS
DEC 21, 2022

https://lims.tagleaf.com/coa_/KHY0hEQIjN

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OMP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED.

END OF REPORT




CERTIFICATE OF ANALYSIS

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

H.23.006.BIN-PEST (TINCTURE) // PRODUCED: JUL 25, 2023

CLIENT: HEALER HEMP LLC // BATCH: PASS



BATCH NO.: H.23.006 ¹
MATRIX: TINCTURE ¹
SAMPLE ID: NAL-230721-018
COLLECTED ON: JUL 21, 2023
RECEIVED ON: JUL 21, 2023
SAMPLE SIZE: 2.688 G ¹
SAMPLED BY: ANNA KUPEL
RECEIVED BY: IAN LEONARD

¹ ENTERED BY CLIENT



NOVA ANALYTIC LABS
 Tomorrow's Testing, Today.

MANUFACTURER INFO

MANUFACTURER
 HEALER HEMP LLC
 119 ORION ST
 BRUNSWICK, MAINE 04011

LICENSE
 CGR26424
 MEDICINAL - CAREGIVER

BATCH RESULT: PASS

PESTICIDES TESTED

: PESTICIDES, INSECTICIDES, FUNGICIDES AND GROWTH REGULATORS BY LC-HRMS
PREPARATION: JUL 24, 2023 // ANALYSIS: JUL 24, 2023


ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
NALED	500 µg/kg	ND	139/186	N/A
OXAMYL	1000 µg/kg	ND	139/465	N/A
PHOSMET	200 µg/kg	ND	139/139	N/A
ACEPHATE	400 µg/kg	ND	139/186	N/A
ALDICARB	400 µg/kg	ND	139/186	N/A
BOSCALID	400 µg/kg	ND	139/186	N/A
CARBARYL	200 µg/kg	ND	139/139	N/A
DIAZINON	200 µg/kg	ND	139/139	N/A
FIPRONIL	400 µg/kg	ND	139/186	N/A
IMAZALIL	200 µg/kg	ND	139/139	N/A
METHOMYL	400 µg/kg	ND	139/186	N/A
PROPOXUR	200 µg/kg	ND	139/139	N/A
SPINOSAD	200 µg/kg	ND	139/139	N/A
ABAMECTIN	500 µg/kg	ND	139/186	N/A
ETOXAZOLE	200 µg/kg	ND	139/139	N/A
MGK-264 I		ND	85.0/85.0	N/A
MALATHION	200 µg/kg	ND	139/139	N/A
METALAXYL	200 µg/kg	ND	139/139	N/A
PYRIDABEN	200 µg/kg	ND	139/139	N/A
BIFENAZATE	200 µg/kg	ND	139/139	N/A
BIFENTHRIN	200 µg/kg	ND	139/139	N/A
CARBOFURAN	200 µg/kg	ND	139/139	N/A
CYFLUTHRIN	1000 µg/kg	ND	139/465	N/A
DAMINOZIDE	1000 µg/kg	ND	139/465	N/A
DICHLORVOS	1000 µg/kg	ND	139/465	N/A
DIMETHOATE	200 µg/kg	ND	139/139	N/A
ETOFENPROX	400 µg/kg	ND	139/186	N/A
FENOXICARB	200 µg/kg	ND	139/139	N/A
FLONICAMID	1000 µg/kg	ND	139/465	N/A
MGK-264 II		ND	54.3/54.3	N/A
METHIOCARB	200 µg/kg	ND	139/139	N/A
ACEQUINOCYL	2000 µg/kg	ND	139/929	N/A

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
ETHOPROPHOS	200 µg/kg	ND	139/139	N/A
FLUDIOXONIL	400 µg/kg	ND	139/186	N/A
HEXYTHIAZOX	1000 µg/kg	ND	139/465	N/A
PRALLETHRIN	200 µg/kg	ND	139/139	N/A
SPIROXAMINE	400 µg/kg	ND	139/186	N/A
THIACLOPRID	200 µg/kg	ND	139/139	N/A
AZOXYSTROBIN	200 µg/kg	ND	139/139	N/A
CHLORFENAPYR	1000 µg/kg	ND	139/465	N/A
CHLORPYRIFOS	200 µg/kg	ND	139/139	N/A
CLOFENTEZINE	200 µg/kg	ND	139/139	N/A
CYPERMETHRIN	1000 µg/kg	ND	139/465	N/A
IMIDACLOPRID	400 µg/kg	ND	139/186	N/A
MYCLOBUTANIL	200 µg/kg	ND	139/139	N/A
SPIROMESIFEN	200 µg/kg	ND	139/139	N/A
TEBUCONAZOLE	400 µg/kg	ND	139/186	N/A
THIAMETHOXAM	200 µg/kg	ND	139/139	N/A
FENPYROXIMATE	400 µg/kg	ND	139/186	N/A
PACLOBUTRAZOL	400 µg/kg	ND	139/186	N/A
PROPICONAZOLE	400 µg/kg	ND	139/186	N/A
SPIROTETRAMAT	200 µg/kg	ND	139/139	N/A
PERMETHRIN CIS		ND	59.9/59.9	N/A
KRESOXIM-METHYL	400 µg/kg	ND	139/186	N/A
TRIFLOXYSTROB-IN	200 µg/kg	ND	139/139	N/A
PARATHION-METHYL	200 µg/kg	ND	139/139	N/A
PERMETHRIN TRANS		ND	79.4/79.4	N/A
PIPERONYLBUTO-XIDE	2000 µg/kg	ND	139/929	N/A

ACETAMIPRID	200 µg/kg	ND	139/139	N/A	CHLORANTRANIL-IPROLE	200 µg/kg	ND	139/139	N/A
					PYRETHRINS CINERIN I		ND	92.8/92.8	N/A
					PYRETHRINS CINERIN II		ND	94.8/94.8	N/A
					PYRETHRINS JASMOLIN I		ND	75.3/75.3	N/A
					PYRETHRINS JASMOLIN II		ND	58.5/58.5	N/A
					PYRETHRINS PYRETHRIN I		ND	432/432	N/A
					PYRETHRINS PYRETHRIN II		ND	255/255	N/A



AUTHORIZED BY:
ZACHARY SMITH
LABORATORY MANAGER, NOVA
ANALYTIC LABS
JUL 25, 2023



** FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.*

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OCP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED. THIS CERTIFICATE OF ANALYSIS IS RELEVANT ONLY TO THOSE ITEMS TESTED. THE SAMPLE WAS PROVIDED TO THE LABORATORY FOR TESTING BY THE CLIENT AND THE SAMPLE WAS TESTED AS RECEIVED.

END OF REPORT




CERTIFICATE OF ANALYSIS

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

H.23.006.BIN-METALS (TINCTURE) // PRODUCED: JUL 25, 2023

CLIENT: HEALER HEMP LLC // BATCH: PASS



BATCH NO.: H.23.006 ¹
MATRIX: TINCTURE ¹
SAMPLE ID: NAL-230721-019
COLLECTED ON: JUL 21, 2023
RECEIVED ON: JUL 21, 2023
SAMPLE SIZE: 2.668 G ¹
SAMPLED BY: ANNA KUPEL
RECEIVED BY: IAN LEONARD

¹ ENTERED BY CLIENT



NOVA ANALYTIC LABS
Tomorrow's Testing, Today.

MANUFACTURER INFO

MANUFACTURER
HEALER HEMP LLC
119 ORION ST
BRUNSWICK, MAINE 04011

LICENSE
CGR26424
MEDICINAL - CAREGIVER

BATCH RESULT: PASS

METALS PASS

HME.1: HEAVY METALS BY ICP-MS PREPARATION: JUL 24, 2023 // ANALYSIS: JUL 25, 2023

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
ARSENIC	1500 µg/kg	ND	10.0/84.1	PASS
CADMIUM	500 µg/kg	ND	4.34/84.1	PASS

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
LEAD	500 µg/kg	ND	4.64/101	PASS
MERCURY	3000 µg/kg	ND	15.5/67.3	PASS



AUTHORIZED BY:
ZACHARY SMITH
LABORATORY MANAGER, NOVA
ANALYTIC LABS
JUL 25, 2023

* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OCP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED. THIS CERTIFICATE OF ANALYSIS IS RELEVANT ONLY TO THOSE ITEMS TESTED. THE SAMPLE WAS PROVIDED TO THE LABORATORY FOR TESTING BY THE CLIENT AND THE SAMPLE WAS TESTED AS RECEIVED.

END OF REPORT