



## Healer Products Certificates of Analysis (COA)

Dear Healer Patron,

We are committed to producing high quality, clean, and accurately labeled cannabis products to help you feel your best. As you'll see in the following pages, we invest in the most thorough testing available in our region, not just for the content of medicinal components, but also for the absence of pesticides, toxic solvents, heavy metals, and microbiological contaminants.

To be transparent and earn your trust, our third-party laboratory certificates of analysis are attached.

Having previously owned and participated in a cannabis analytic laboratory for several years, I understand the inherent challenges related to reproducibility, calibration, and validation with peer laboratories. In the cannabis analytic industry, potency results are considered accurate within 10% deviation from the actual value. That's why after Healer performs its own internal analytics, we send samples of our bulk extracts and final products to at least one third-party lab, and sometimes two.

If you have any questions about the data on the following pages, we'd love to hear from you. Thank you for choosing Healer and taking a powerful step for your good health.

Sincerely,

Dr. Dustin Sulak

## CANNABINOIDS

Cannabinoid	Concentration	
	mg/g	mg/Capsule*
<b>TOTAL</b>	<b>29.42</b>	<b>10.30</b>
CBC	1.70	0.60
CBCA	0.21	0.07
CBD	2.87	1.00
CBDA	1.48	0.52
CBDV		
CBDVA		
CBG	19.20	6.72
CBGA	3.64	1.27
CBL		
CBLA		
CBN		
CBNA		
$\Delta^8$ -THC		
$\Delta^9$ -THC	0.32	0.11
$\Delta^{10}$ -THC		
EXO-THC		
THCA		
THCV		
THCVA		
3 <sup>rd</sup> Party Tested By:	Nova Analytic Labs	
3 <sup>rd</sup> Party Testing ID:	CBG.C.23.003-Syloid-Cann NAL-230818-003	

\*Capsule weight of 0.35g

**Product Type:**  
CBG Capsules

**Batch ID:**  
CBG.C.23.003

**Product Expiration Date:**  
August 28, 2025

**COA Issue Date:**  
August 29, 2023

**Ingredients:**

Organic MCT Coconut Oil, Organic  
Maine Hemp <0.3% THC, Traces of  
Ethyl Alcohol (Ethanol),  
Pharmaceutical Grade Syloid  
(Amorphous Silicon-Dioxide),  
Vegetarian HPMC Capsules

**Strains:**

Sour G, Forbidden V, Sour Elektra, Suver  
Haze, Lifter, Sour Space Candy, Sour  
Hawaiian Haze

# Whole Plant Hemp CBG Capsules

Batch ID: CBG.C.23.003



TEST	RESULTS
Ethanol	Pass-1640µg/g Detected (1.64 mg/g)
3 <sup>rd</sup> Party Tested By:	Nova Analytic Labs
3 <sup>rd</sup> Party Testing ID:	CBG.C.23.003-Solv NAL-230823-016
*For full list of solvents see attached	

**MICROBIOLOGICAL CONTAMINANTS**

TEST	RESULTS
Enterobacter	Pass-None Detected
Coliform	Pass-None Detected
Aerobic Bacteria	Pass-None Detected
Yeast and Mold	Pass-None Detected
Salmonella	Pass-None Detected
E.Coli	Pass-None Detected
3 <sup>rd</sup> Party Tested By:	Nova Analytic Labs
3 <sup>rd</sup> Party Testing ID:	CBG.C.23.003-Micro NAL-230823-014

**HEAVY METALS**

TEST	RESULTS
Arsenic	Pass- <LOQ
Cadmium	Pass-None Detected
Lead	Pass-None Detected
Mercury	Pass-None Detected
3 <sup>rd</sup> Party Tested By:	Nova Analytic Labs
3 <sup>rd</sup> Party Testing ID:	H.22.CBDA.Bulk-Metals, H.23.006.Bin-Metals NAL-230302-002, NAL-230721-019
*Bulk concentrate tested*	

**PESTICIDES**

TEST	RESULTS
Bifenthrin	Pass-None Detected
Cyfluthrin	Pass-None Detected
Daminozide	Pass-None Detected
Etoxazole	Pass-None Detected
Imazalil	Pass-None Detected
Myclobutanil	Pass-None Detected
Spiromesifen	Pass-None Detected
Trifloxystrobin	Pass-None Detected
3 <sup>rd</sup> Party Tested By:	Nova Analytic Labs
3 <sup>rd</sup> Party Testing ID:	H.22.CBDA.Bulk-Pest, H.23.006.Bin-Pest NAL-230302-003, NAL-230721-016
*Bulk concentrate tested	

## TERPENES

Terpene	Concentration	
	mg/g	mg/Capsule*
<b>TOTAL</b>	<b>1.430</b>	<b>0.501</b>
$\beta$ -Caryophyllene	0.677	0.237
$\alpha$ -Humulene	<LOQ	<LOQ
D-Limonene		
$\alpha$ -Pinene		
$\beta$ -Myrcene		
$\beta$ -Pinene		
Linalool		
Camphene		
$\alpha$ -Bisabolol	0.462	0.162
$\gamma$ -Terpinene		
Terpinolene		
P-Cymene		
Isopulegol		
Guaiol	0.291	0.102
Cis-Nerolidol		
Eucalyptol		
$\Delta^3$ -Carene		
Caryophyllene Oxide		
$\beta$ -Ocimene		
$\alpha$ -Terpinene		
$\alpha$ -Ocimene		
Trans-Nerolidol		
3 <sup>rd</sup> Party Tested By:	Nova Analytic Labs	
3 <sup>rd</sup> Party Testing ID:	CBG.C.23.003-Terps NAL-230823-013	

\*\*<LOQ = Compound present in detectable  
amounts below the limit of quantitation  
for data reporting.

**MYCOTOXINS**

TEST	RESULTS
Aflatoxin B1, B2, G1, G2	Pass-None Detected
Ochratoxin A	Pass- None Detected
3 <sup>rd</sup> Party Tested By:	Nova Analytic Labs
3 <sup>rd</sup> Party Testing ID:	CBG.C.23.003-Myco NAL-230823-015

**3<sup>rd</sup> Party  
Lab Results  
Attached**



# CERTIFICATE OF ANALYSIS

\* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

**CBG.C.23.003-SYLOID-CANN (EDIBLE SOLID) // PRODUCED: AUG 21, 2023**

**CLIENT: HEALER HEMP LLC // BATCH: PASSED**



**BATCH NO.:** CBG.C.23.003 <sup>1</sup>  
**MATRIX:** EDIBLE SOLID <sup>1</sup>  
**SAMPLE ID:** NAL-230818-003  
**COLLECTED ON:** AUG 18, 2023  
**RECEIVED ON:** AUG 18, 2023  
**SAMPLE SIZE:** 2.928 G <sup>1</sup>  
**SAMPLED BY:** ANNA KUPEL  
**RECEIVED BY:** IAN LEONARD  
**SERVING SIZE:** .35 G <sup>1</sup>

<sup>1</sup> ENTERED BY CLIENT

## CANNABINOID OVERVIEW

**CBG:** 6.72 mg/srv  
**CBGA:** 1.27 mg/srv  
**TOTAL CANNABINOIDS:** 10.3 mg/srv

## MANUFACTURER INFO

**MANUFACTURER**  
 HEALER HEMP LLC  
 119 ORION ST  
 BRUNSWICK, MAINE 04011  
**LICENSE**  
 CGR26424  
 MEDICINAL - CAREGIVER

## BATCH RESULT: PASSED

**POTENCY** PASS

## CAN.1: POTENCY & CANNABINOID PROFILE BY HPLC-UV PREPARATION: AUG 18, 2023, AUG 21, 2023 // ANALYSIS: AUG 21, 2023

ANALYTE	LIMIT	AMT	AMT	LOD/LOQ (%)	PASS/FAIL	ANALYTE	LIMIT	AMT	AMT	LOD/LOQ (%)	PASS/FAIL
CBC	0.170 %	1.70 mg/g	0.000567/0.00284	N/A		Δ <sup>8</sup> -THCA	ND	ND	0.000567/0.00284	N/A	
CBCA	0.0210 %	0.210 mg/g	0.000567/0.00284	N/A		Δ <sup>9</sup> -THC	0.0324 %	0.324 mg/g	0.000567/0.00284	N/A	
CBD	0.287 %	2.87 mg/g	0.000567/0.00284	N/A		Δ <sup>10</sup> -THC	ND	ND	0.000567/0.00284	N/A	
CBDA	0.148 %	1.48 mg/g	0.000567/0.00284	N/A		EXO-THC	ND	ND	0.000567/0.00284	N/A	
CBDV	ND	ND	0.000567/0.00284	N/A		THCA	ND	ND	0.000567/0.00284	N/A	
CBDVA	ND	ND	0.000567/0.00284	N/A		THCV	ND	ND	0.000567/0.00284	N/A	
CBG	1.92 %	19.2 mg/g	0.00630/0.0315	N/A		THCVA	ND	ND	0.000567/0.00284	N/A	
CBGA	0.364 %	3.64 mg/g	0.000567/0.00284	N/A		TOTAL THC**	0.0324 %	0.324 mg/g		N/A	
CBL	ND	ND	0.000567/0.00284	N/A		TOTAL CBD**	0.417 %	4.17 mg/g		N/A	
CBLA	ND	ND	0.000567/0.00284	N/A		CBD/SRV	1.00 mg			N/A	
CBN	ND	ND	0.000567/0.00284	N/A		Δ <sup>9</sup> -THC/SRV	0.113 mg			N/A	
CBNA	ND	ND	0.000567/0.00284	N/A		TOTAL THC/SRV**	0.113 mg			N/A	
Δ <sup>8</sup> -THC	ND	ND	0.000567/0.00284	N/A		TOTAL CBD/SRV**	1.46 mg			N/A	

\*\* TOTAL CBD = (CBDA X 0.877) + CBD


\*\* TOTAL THC = (THCA X 0.877) + THC

Reported on an as received basis

1000 µg/g = 1 mg/g



**AUTHORIZED BY:**  
 ZACHARY SMITH  
 LABORATORY MANAGER, NOVA  
 ANALYTIC LABS  
 AUG 21, 2023



[https://lims.tagleaf.com/coa\\_bMs99y6ll1](https://lims.tagleaf.com/coa_bMs99y6ll1)

NOTES


ZACHARY SMITH  
AUG 21, 2023

POTENCY & CANNABINOID PROFILE BY HPLC-UV  
THE STANDARD LAB UNCERTAINTY FOR POTENCY IS 5% OF THE REPORTED VALUE.

*\* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.*

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OCP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED, THIS CERTIFICATE OF ANALYSIS IS RELEVANT ONLY TO THOSE ITEMS TESTED. THE SAMPLE WAS PROVIDED TO THE LABORATORY FOR TESTING BY THE CLIENT AND THE SAMPLE WAS TESTED AS RECEIVED.

END OF REPORT

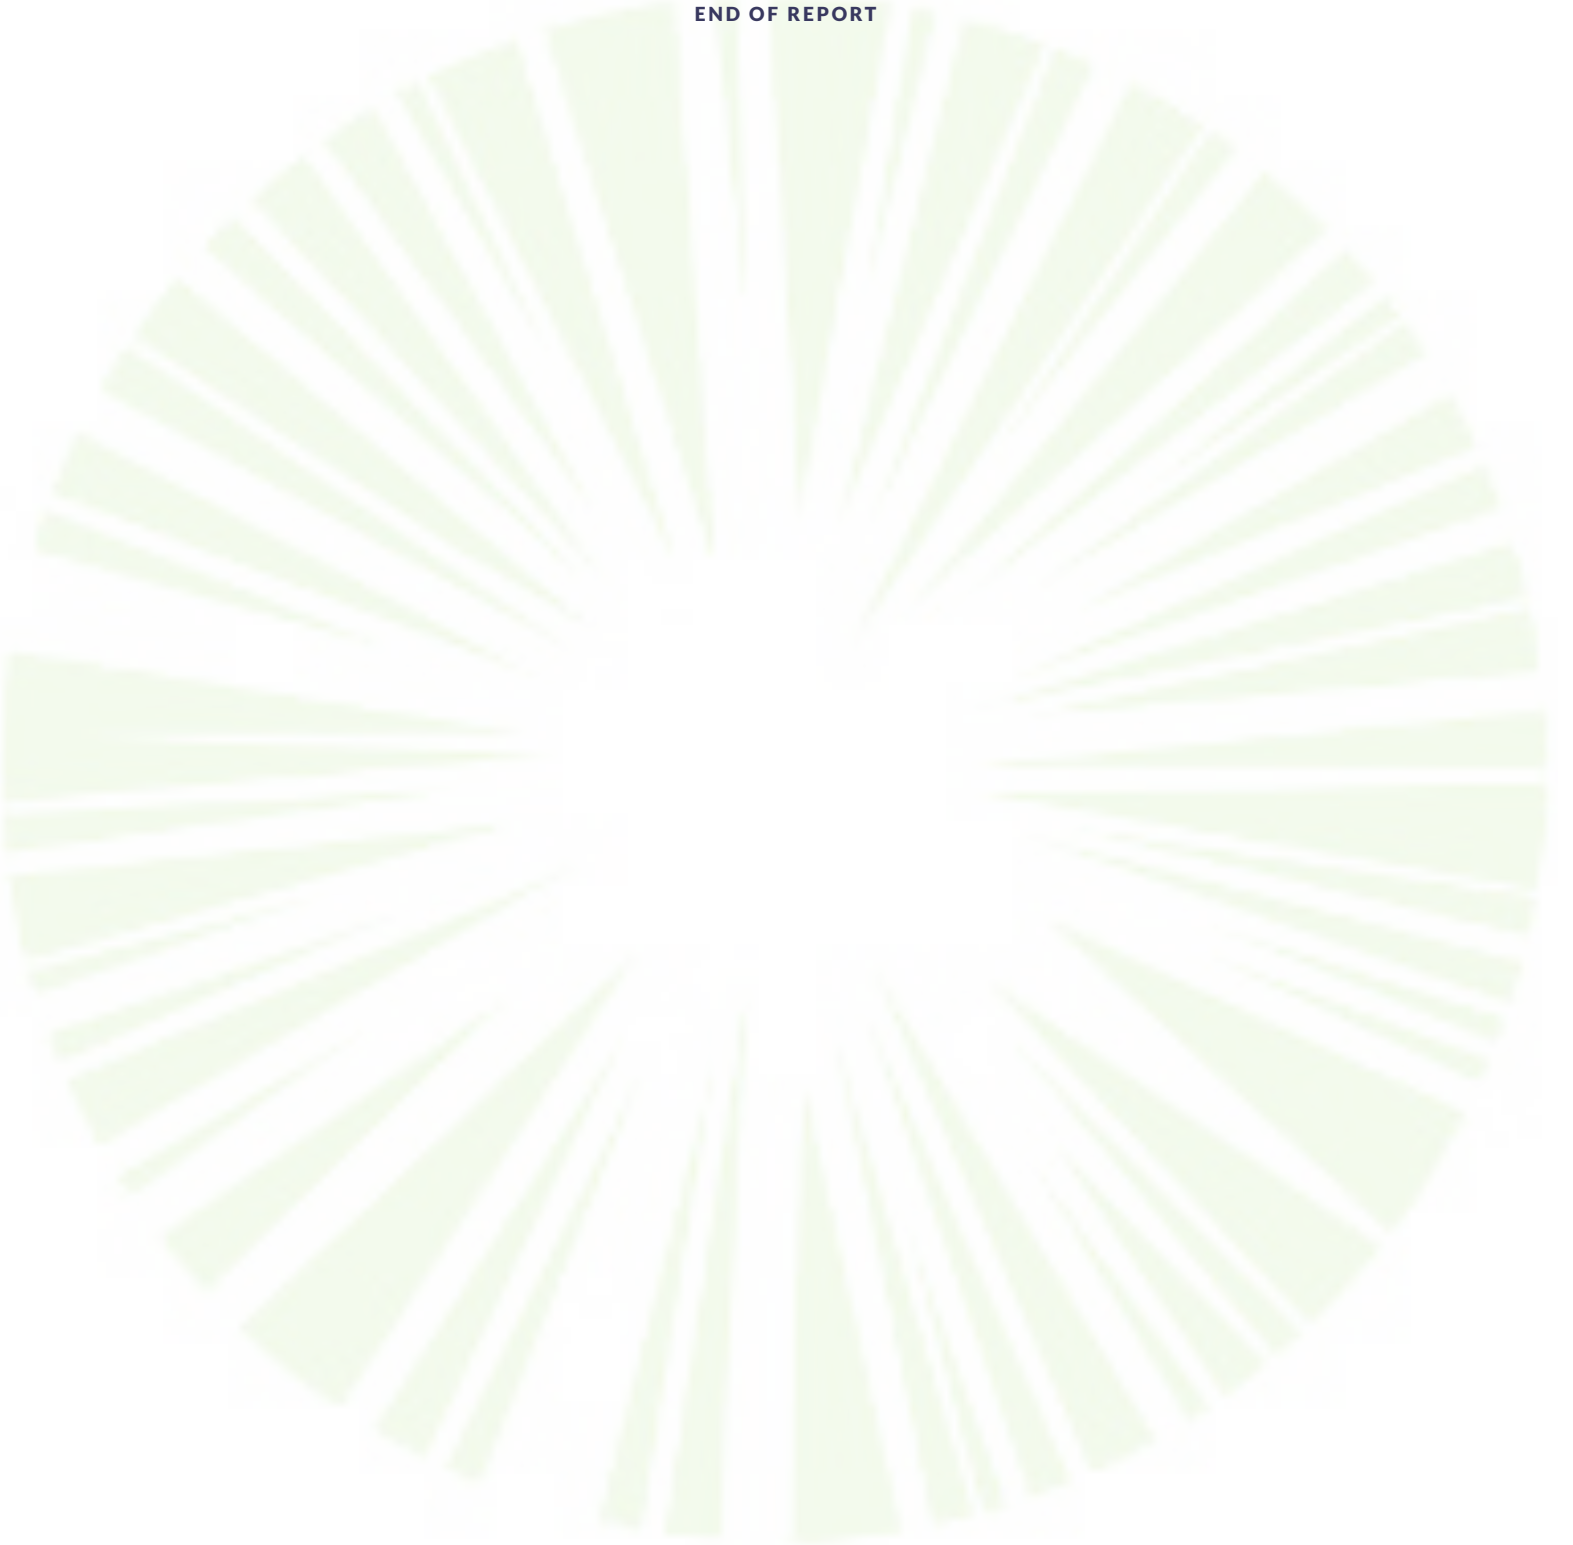


## CERTIFICATE OF ANALYSIS

\* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

**CBG.C.23.003-TERPS (EDIBLE SOLID) // PRODUCED: AUG 29, 2023**

**CLIENT: HEALER HEMP LLC // BATCH: PASSED**



**BATCH NO.:** CBG.C.23.003 <sup>1</sup>  
**MATRIX:** EDIBLE SOLID <sup>1</sup>  
**SAMPLE ID:** NAL-230823-013  
**COLLECTED ON:** AUG 23, 2023  
**RECEIVED ON:** AUG 23, 2023  
**SAMPLE SIZE:** 1.939 G <sup>1</sup>  
**SAMPLED BY:** ANNA KUPEL  
**RECEIVED BY:** TORI DANIS

<sup>1</sup> ENTERED BY CLIENT



**NOVA ANALYTIC LABS**  
 Tomorrow's Testing, Today.

### MANUFACTURER INFO

**MANUFACTURER**  
 HEALER HEMP LLC  
 119 ORION ST  
 BRUNSWICK, MAINE 04011

**LICENSE**  
 CGR26424  
 MEDICINAL - CAREGIVER

### BATCH RESULT: PASSED

**TERPENES** TESTED

### TRP.2: TERPENES BY LIQUID INJECT GCMS PREPARATION: AUG 26, 2023 // ANALYSIS: AUG 26, 2023

ANALYTE	AMT	AMT	LOD/LOQ (mg/g)	PASS/FAIL
<b>TOTAL TERPENES</b>	0.143 %	1.43 mg/g		N/A
<b>NEROL</b>	ND	ND	0.132/0.265	N/A
<b>CEDROL</b>	ND	ND	0.132/0.265	N/A
<b>CITRAL</b>	ND	ND	0.132/0.265	N/A
<b>GUAJOL</b>	0.0291 %	0.291 mg/g	0.132/0.265	N/A
<b>THYMOL</b>	ND	ND	0.132/0.265	N/A
<b>BORNEOL</b>	ND	ND	0.132/0.265	N/A
<b>CAMPHOR</b>	ND	ND	0.132/0.265	N/A
<b>MENTHOL</b>	ND	ND	0.132/0.265	N/A
<b>PHYTANE</b>	ND	ND	0.132/0.265	N/A
<b>CAMPHENE</b>	ND	ND	0.132/0.265	N/A
<b>FARNESOL</b>	ND	ND	0.132/0.265	N/A
<b>FENCHONE</b>	ND	ND	0.132/0.265	N/A
<b>GERANIOL</b>	ND	ND	0.132/0.265	N/A
<b>LINALOOL</b>	ND	ND	0.132/0.265	N/A
<b>MENTHONE</b>	ND	ND	0.132/0.265	N/A
<b>PULEGONE</b>	ND	ND	0.132/0.265	N/A
<b>SABINENE</b>	ND	ND	0.132/0.265	N/A
<b>SAFRANAL</b>	ND	ND	0.132/0.265	N/A
<b>M-CYMENE</b>	ND	ND	0.132/0.265	N/A
<b>O-CYMENE</b>	ND	ND	0.132/0.265	N/A
<b>P-CYMENE</b>	ND	ND	0.132/0.265	N/A
<b>CARVACROL</b>	ND	ND	0.132/0.265	N/A
<b>FARNESENE</b>	ND	ND	0.132/0.265	N/A
<b>TERPINEOL</b>	ND	ND	0.132/0.265	N/A
<b>VALENCENE</b>	ND	ND	0.132/0.265	N/A
<b>D-CARVONE</b>	ND	ND	0.132/0.265	N/A
<b>EUCALYPTOL</b>	ND	ND	0.132/0.265	N/A
<b>ISOBORNEOL</b>	ND	ND	0.132/0.265	N/A
<b>ISOPULEGOL</b>	ND	ND	0.132/0.265	N/A

ANALYTE	AMT	AMT	LOD/LOQ (mg/g)	PASS/FAIL
<b>PIPERITONE</b>	ND	ND	0.132/0.265	N/A
<b>D-LIMONENE</b>	ND	ND	0.132/0.265	N/A
<b>CITRONELLOL</b>	ND	ND	0.132/0.265	N/A
<b>E-NEROLIDOL</b>	ND	ND	0.132/0.265	N/A
<b>TERPINOLENE</b>	ND	ND	0.132/0.265	N/A
<b>Z-NEROLIDOL</b>	ND	ND	0.132/0.265	N/A
<b>β-PINENE</b>	ND	ND	0.132/0.265	N/A
<b>2-PIPERIDONE</b>	ND	ND	0.132/0.265	N/A
<b>α-PINENE</b>	ND	ND	0.132/0.265	N/A
<b>β-MYRCENE</b>	ND	ND	0.132/0.265	N/A
<b>(-)-VERBENONE</b>	ND	ND	0.132/0.265	N/A
<b>OCTYL ACETATE</b>	ND	ND	0.132/0.265	N/A
<b>TERPINEN-4-OL</b>	ND	ND	0.132/0.265	N/A
<b>α-CEDRENE</b>	ND	ND	0.132/0.265	N/A
<b>α-THUJONE</b>	ND	ND	0.132/0.265	N/A
<b>Δ<sup>3</sup>-CARENE</b>	ND	ND	0.132/0.265	N/A
<b>α-HUMULENE</b>	< LOQ	< LOQ	0.132/0.265	N/A
<b>GERANYL ACETATE</b>	ND	ND	0.132/0.265	N/A
<b>α-BISABOLOL</b>	0.0462 %	0.462 mg/g	0.132/0.265	N/A
<b>α-TERPINENE</b>	ND	ND	0.132/0.265	N/A
<b>γ-TERPINENE</b>	ND	ND	0.132/0.265	N/A
<b>SABINENE HYDRATE</b>	ND	ND	0.132/0.265	N/A
<b>CIS-β-OCIMENE</b>	ND	ND	0.132/0.265	N/A
<b>ISOBORNYL ACETATE</b>	ND	ND	0.132/0.265	N/A
<b>α-PHELLANDRENE</b>	ND	ND	0.132/0.265	N/A
<b>β-CARYOPHYLLENE</b>	0.0677 %	0.677 mg/g	0.132/0.265	N/A
<b>TRANS-β-OCIMENE</b>	ND	ND	0.132/0.265	N/A
<b>CARYOPHYLLENE OXIDE</b>	ND	ND	0.132/0.265	N/A
<b>ENDO FENCHYL ALCOHOL</b>	ND	ND	0.132/0.265	N/A





[https://lims.tagleaf.com/coa\\_/ohieYLZiYT](https://lims.tagleaf.com/coa_/ohieYLZiYT)

*\* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.*

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OCP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED. THIS CERTIFICATE OF ANALYSIS IS RELEVANT ONLY TO THOSE ITEMS TESTED. THE SAMPLE WAS PROVIDED TO THE LABORATORY FOR TESTING BY THE CLIENT AND THE SAMPLE WAS TESTED AS RECEIVED.

**END OF REPORT**




## CERTIFICATE OF ANALYSIS

\* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

**CBG.C.23.003-MICRO (EDIBLE SOLID) // PRODUCED: AUG 28, 2023**

**CLIENT: HEALER HEMP LLC // BATCH: PASSED**



**BATCH NO.:** CBG.C.23.003 <sup>1</sup>  
**MATRIX:** EDIBLE SOLID <sup>1</sup>  
**SAMPLE ID:** NAL-230823-014  
**COLLECTED ON:** AUG 23, 2023  
**RECEIVED ON:** AUG 23, 2023  
**SAMPLE SIZE:** 2.39 G <sup>1</sup>  
**SAMPLED BY:** ANNA KUPEL  
**RECEIVED BY:** TORI DANIS

<sup>1</sup> ENTERED BY CLIENT



**NOVA ANALYTIC LABS**  
Tomorrow's Testing, Today.

### MANUFACTURER INFO

**MANUFACTURER**  
HEALER HEMP LLC  
119 ORION ST  
BRUNSWICK, MAINE 04011

**LICENSE**  
CGR26424  
MEDICINAL - CAREGIVER

**BATCH RESULT:** PASSED

**MICROBIAL** TESTED



**AUTHORIZED BY:**  
ZACHARY SMITH  
LABORATORY MANAGER, NOVA  
ANALYTIC LABS  
AUG 28, 2023

[https://lims.tagleaf.com/coa/\\_ciYcjV8rhZ](https://lims.tagleaf.com/coa/_ciYcjV8rhZ)

MIC.3: TOTAL COLIFORM BY MOST PROBABLE NUMBER  
PREPARATION: AUG 23, 2023 // ANALYSIS: AUG 24, 2023

ANALYTE	LIMIT	AMT (CFU/g)	LOD/LOQ (CFU/g)	PASS/FAIL
COLIFORMS	1000 CFU/g	ND	100/100	N/A

MIC.6: TOTAL ENTEROBACTER BY MOST PROBABLE NUMBER  
PREPARATION: AUG 23, 2023 // ANALYSIS: AUG 24, 2023

ANALYTE	LIMIT	AMT (CFU/g)	LOD/LOQ (CFU/g)	PASS/FAIL
ENTEROBACTERIACEAE	1000 CFU/g	ND	100/100	N/A

TOTAL AEROBIC BACTERIA BY MOST PROBABLE NUMBER  
PREPARATION: AUG 23, 2023 // ANALYSIS: AUG 24, 2023

ANALYTE	LIMIT	AMT (CFU/g)	LOD/LOQ (CFU/g)	PASS/FAIL
AEROBIC BACTERIA	100000 CFU/g	ND	100/100	N/A

MIC.5: SALMONELLA BY PCR  
PREPARATION: AUG 23, 2023 // ANALYSIS: AUG 24, 2023

ANALYTE	LIMIT	AMT (CFU/g)	LOD/LOQ (CFU/g)	PASS/FAIL
SALMONELLA SPP.	Any amt in 1 gram	ND	1.00/1.00	N/A

MIC.4: PATHOGENIC E. COLI BY PCR  
PREPARATION: AUG 23, 2023 // ANALYSIS: AUG 24, 2023

ANALYTE	LIMIT	AMT (CFU/g)	LOD/LOQ (CFU/g)	PASS/FAIL
SHIGA TOXIN-PRODUCING E. COLI	Any amt in 1 gram	ND	1.00/1.00	N/A

TOTAL YEAST AND MOLD BY MOST PROBABLE NUMBER  
PREPARATION: AUG 23, 2023 // ANALYSIS: AUG 26, 2023

ANALYTE	LIMIT	AMT (CFU/g)	LOD/LOQ (CFU/g)	PASS/FAIL
YEAST & MOLD	10000 CFU/g	ND	100/100	N/A

\* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OCP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED. THIS CERTIFICATE OF ANALYSIS IS RELEVANT ONLY TO THOSE ITEMS TESTED. THE SAMPLE WAS PROVIDED TO THE LABORATORY FOR TESTING BY THE CLIENT AND THE SAMPLE WAS TESTED AS RECEIVED.

END OF REPORT






## CERTIFICATE OF ANALYSIS

\* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

**CBG.C.23.003-MYCO (EDIBLE SOLID) // PRODUCED: AUG 25, 2023**

**CLIENT: HEALER HEMP LLC // BATCH: PASSED**



**BATCH NO.:** CBG.C.23.003 <sup>1</sup>  
**MATRIX:** EDIBLE SOLID <sup>1</sup>  
**SAMPLE ID:** NAL-230823-015  
**COLLECTED ON:** AUG 23, 2023  
**RECEIVED ON:** AUG 23, 2023  
**SAMPLE SIZE:** 2.035 G <sup>1</sup>  
**SAMPLED BY:** ANNA KUPEL  
**RECEIVED BY:** TORI DANIS

<sup>1</sup> ENTERED BY CLIENT



**NOVA ANALYTIC LABS**  
Tomorrow's Testing, Today.

### MANUFACTURER INFO

**MANUFACTURER**  
HEALER HEMP LLC  
119 ORION ST  
BRUNSWICK, MAINE 04011

**LICENSE**  
CGR26424  
MEDICINAL - CAREGIVER

**BATCH RESULT:** PASSED

**MYCOTOXINS** TESTED

**MYC.1: MYCOTOXINS BY LC-HRMS**  
**PREPARATION: AUG 24, 2023 // ANALYSIS: AUG 24, 2023**

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
AFLATOXIN B1		ND	0.104/0.313	N/A
AFLATOXIN B2		ND	0.313/0.521	N/A
AFLATOXIN G1		ND	0.104/0.313	N/A

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
AFLATOXIN G2		ND	0.104/0.521	N/A
OCHRATOXIN A		ND	0.209/0.626	N/A



**AUTHORIZED BY:**  
ZACHARY SMITH  
LABORATORY MANAGER, NOVA  
ANALYTIC LABS  
AUG 25, 2023

[https://lims.tagleaf.com/coa\\_/A0LPHZOKQR](https://lims.tagleaf.com/coa_/A0LPHZOKQR)

\* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OCP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED. THIS CERTIFICATE OF ANALYSIS IS RELEVANT ONLY TO THOSE ITEMS TESTED. THE SAMPLE WAS PROVIDED TO THE LABORATORY FOR TESTING BY THE CLIENT AND THE SAMPLE WAS TESTED AS RECEIVED.


**END OF REPORT**

## CERTIFICATE OF ANALYSIS

\* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

**CBG.C.23.003-SOLV (EDIBLE SOLID) // PRODUCED: AUG 25, 2023**

**CLIENT: HEALER HEMP LLC // BATCH: PASSED**



**BATCH NO.:** CBG.C.23.003 <sup>1</sup>  
**MATRIX:** EDIBLE SOLID <sup>1</sup>  
**SAMPLE ID:** NAL-230823-016  
**COLLECTED ON:** AUG 23, 2023  
**RECEIVED ON:** AUG 23, 2023  
**SAMPLE SIZE:** 1.435 G <sup>1</sup>  
**SAMPLED BY:** ANNA KUPEL  
**RECEIVED BY:** TORI DANIS

<sup>1</sup> ENTERED BY CLIENT



**NOVA ANALYTIC LABS**  
 Tomorrow's Testing, Today.

### MANUFACTURER INFO

**MANUFACTURER**  
 HEALER HEMP LLC  
 119 ORION ST  
 BRUNSWICK, MAINE 04011

**LICENSE**  
 CGR26424  
 MEDICINAL - CAREGIVER

### BATCH RESULT: PASSED

**SOLVENTS** TESTED

### RSOL.1: RESIDUAL SOLVENTS, POISONS AND TOXINS BY HEADSPACE GC-MS PREPARATION: AUG 24, 2023 // ANALYSIS: AUG 25, 2023

ANALYTE	LIMIT	AMT (µg/g)	LOD/LOQ (µg/g)	PASS/FAIL
BUTANE	5000 µg/g	ND	0.993/2.48	N/A
HEXANE	290 µg/g	ND	0.993/2.48	N/A
ACETONE	5000 µg/g	ND	49.6/99.3	N/A
BENZENE	1 µg/g	ND	0.496/0.993	N/A
ETHANOL	5000 µg/g	1640	19.9/49.6	N/A
HEPTANE	5000 µg/g	ND	9.93/19.9	N/A
PENTANE	5000 µg/g	ND	9.93/19.9	N/A
PROPANE	5000 µg/g	ND	19.9/39.7	N/A
TOLUENE	890 µg/g	ND	4.96/9.93	N/A
METHANOL	3000 µg/g	ND	49.6/99.3	N/A
O-XYLENE	2170 µg/g	ND	9.93/19.9	N/A

ANALYTE	LIMIT	AMT (µg/g)	LOD/LOQ (µg/g)	PASS/FAIL
CHLOROFORM	1 µg/g	ND	0.496/0.993	N/A
ETHYL ETHER	5000 µg/g	ND	9.93/19.9	N/A
ACETONITRILE	410 µg/g	ND	9.93/19.9	N/A
ETHYL ACETATE	5000 µg/g	ND	9.93/19.9	N/A
ETHYLENE OXIDE	1 µg/g	ND	0.496/0.993	N/A
P- AND M-XYLENE	2170 µg/g	ND	19.9/39.7	N/A
ISOPROPYL ALCOHOL	5000 µg/g	ND	49.6/99.3	N/A
TRICHLOROETHYLENE	1 µg/g	ND	0.496/0.993	N/A
1,2-DICHLOROETHANE	1 µg/g	ND	0.496/0.993	N/A
METHYLENE CHLORIDE	1 µg/g	ND	0.496/0.993	N/A



**AUTHORIZED BY:**  
 ZACHARY SMITH  
 LABORATORY MANAGER, NOVA  
 ANALYTIC LABS  
 AUG 25, 2023

<https://lims.tagleaf.com/coa/XtuZ6EGHo2>

\* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OCP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED. THIS CERTIFICATE OF ANALYSIS IS RELEVANT ONLY TO THOSE ITEMS TESTED. THE SAMPLE WAS PROVIDED TO THE LABORATORY FOR TESTING BY THE CLIENT AND THE SAMPLE WAS TESTED AS RECEIVED.


**END OF REPORT**

## CERTIFICATE OF ANALYSIS

\* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

**H.22.CBDA.BULK-METALS (TINCTURE) // PRODUCED: MAR 03, 2023**

**CLIENT: HEALER HEMP LLC // BATCH: PASSED**



**BATCH NO.:** H.22.CBDA.BULK  
**MATRIX:** TINCTURE  
**SAMPLE ID:** NAL-230302-002  
**COLLECTED ON:** MAR 02, 2023  
**RECEIVED ON:** MAR 02, 2023  
**SAMPLE SIZE:** 3.821 G  
**SAMPLED BY:** ANNA KUPEL  
**RECEIVED BY:** CLARA ELIZABETH LUND



**NOVA ANALYTIC LABS**  
Tomorrow's Testing, Today.

### MANUFACTURER INFO

**MANUFACTURER**  
HEALER HEMP LLC  
119 ORION ST  
BRUNSWICK, MAINE 04011

**LICENSE**  
CGR26424  
MEDICINAL - CAREGIVER

**BATCH RESULT:** PASSED

**METALS** TESTED

**HME.1: HEAVY METALS BY ICP-MS**  
**PREPARATION: MAR 02, 2023 // ANALYSIS: MAR 03, 2023**

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
LEAD	500 µg/kg	ND	32.3/97.0	N/A
ARSENIC	1500 µg/kg	ND	32.3/80.8	N/A

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
CADMIUM	500 µg/kg	ND	32.3/80.8	N/A
MERCURY	3000 µg/kg	ND	32.3/64.6	N/A



**RESULTS CERTIFIED BY:**  
BARRY CHAFFIN  
COO, NOVA ANALYTIC LABS  
MAR 03, 2023

**RESULTS CERTIFIED BY:**  
GREG NEWLAND  
CSO, NOVA ANALYTIC LABS  
MAR 03, 2023

**RESULTS CERTIFIED BY:**  
CHRIS ALTOMARE  
CEO, NOVA ANALYTIC LABS  
MAR 03, 2023

[https://lims.tagleaf.com/coa\\_/eNVQ34h7e8](https://lims.tagleaf.com/coa_/eNVQ34h7e8)

\* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OMP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED.

**END OF REPORT**




## CERTIFICATE OF ANALYSIS

\* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

**H.22.CBDA.BULK-PEST (TINCTURE) // PRODUCED: MAR 03, 2023**

**CLIENT: HEALER HEMP LLC // BATCH: PASSED**



**BATCH NO.:** H.22.CBDA.BULK  
**MATRIX:** TINCTURE  
**SAMPLE ID:** NAL-230302-003  
**COLLECTED ON:** MAR 02, 2023  
**RECEIVED ON:** MAR 02, 2023  
**SAMPLE SIZE:** 2.962 G  
**SAMPLED BY:** ANNA KUPEL  
**RECEIVED BY:** CLARA ELIZABETH LUND



**NOVA ANALYTIC LABS**  
Tomorrow's Testing, Today.

### MANUFACTURER INFO

**MANUFACTURER**  
HEALER HEMP LLC  
119 ORION ST  
BRUNSWICK, MAINE 04011

**LICENSE**  
CGR26424  
MEDICINAL - CAREGIVER

### BATCH RESULT: PASSED

**PESTICIDES** TESTED

**: PESTICIDES, INSECTICIDES, FUNGICIDES AND GROWTH REGULATORS BY LC-HRMS**  
**PREPARATION: MAR 02, 2023 // ANALYSIS: MAR 02, 2023**

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
NALED	500 µg/kg	ND	145/194	N/A
OXAMYL	1000 µg/kg	ND	145/485	N/A
PHOSMET	200 µg/kg	ND	145/145	N/A
ACEPHATE	400 µg/kg	ND	145/194	N/A
ALDICARB	400 µg/kg	ND	145/194	N/A
BOSCALID	400 µg/kg	ND	145/194	N/A
CARBARYL	200 µg/kg	ND	145/145	N/A
DIAZINON	200 µg/kg	ND	145/145	N/A
FIPRONIL	400 µg/kg	ND	145/194	N/A
IMAZALIL	200 µg/kg	ND	145/145	N/A
METHOMYL	400 µg/kg	ND	145/194	N/A
PROPOXUR	200 µg/kg	ND	145/145	N/A
SPINOSAD	200 µg/kg	ND	145/145	N/A
ABAMECTIN	500 µg/kg	ND	145/194	N/A
ETOXAZOLE	200 µg/kg	ND	145/145	N/A
MGK-264 I		ND	88.7/88.7	N/A
MALATHION	200 µg/kg	ND	145/145	N/A
METALAXYL	200 µg/kg	ND	145/145	N/A
PYRIDABEN	200 µg/kg	ND	145/145	N/A
BIFENAZATE	200 µg/kg	ND	145/145	N/A
BIFENTHRIN	200 µg/kg	ND	145/145	N/A
CARBOFURAN	200 µg/kg	ND	145/145	N/A
CYFLUTHRIN	1000 µg/kg	ND	145/485	N/A
DAMINOZIDE	1000 µg/kg	ND	145/485	N/A
DICHLORVOS	1000 µg/kg	ND	145/485	N/A
DIMETHOATE	200 µg/kg	ND	145/145	N/A
ETOXENPROX	400 µg/kg	ND	145/194	N/A
FENOXYCARB	200 µg/kg	ND	145/145	N/A
FLONICAMID	1000 µg/kg	ND	145/485	N/A
MGK-264 II		ND	56.7/56.7	N/A
METHIOCARB	200 µg/kg	ND	145/145	N/A
ACEQUINOCYL	2000 µg/kg	ND	145/969	N/A
ACETAMIPRID	200 µg/kg	ND	145/145	N/A

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
ETHOPROPHOS	200 µg/kg	ND	145/145	N/A
FLUDIOXONIL	400 µg/kg	ND	145/194	N/A
HEXYTHIAZOX	1000 µg/kg	ND	145/485	N/A
PRALLETHRIN	200 µg/kg	ND	145/145	N/A
SPIROXAMINE	400 µg/kg	ND	145/194	N/A
THIACLOPRID	200 µg/kg	ND	145/145	N/A
AZOXYSTROBIN	200 µg/kg	ND	145/145	N/A
CHLORFENAPYR	1000 µg/kg	ND	145/485	N/A
CHLORPYRIFOS	200 µg/kg	ND	145/145	N/A
CLOFENTEZINE	200 µg/kg	ND	145/145	N/A
CYPERMETHRIN	1000 µg/kg	ND	145/485	N/A
IMIDACLOPRID	400 µg/kg	ND	145/194	N/A
MYCLOBUTANIL	200 µg/kg	ND	145/145	N/A
SPIROMESIFEN	200 µg/kg	ND	145/145	N/A
TEBUCONAZOLE	400 µg/kg	ND	145/194	N/A
THIAMETHOXAM	200 µg/kg	ND	145/145	N/A
FENPYROXIMATE	400 µg/kg	ND	145/194	N/A
PACLOBUTRAZOL	400 µg/kg	ND	145/194	N/A
PROPICONAZOLE	400 µg/kg	ND	145/194	N/A
SPIROTETRAMAT	200 µg/kg	ND	145/145	N/A
PERMETHRIN CIS		ND	62.5/62.5	N/A
KRESOXIM-METHYL	400 µg/kg	ND	145/194	N/A
TRIFLOXYSTROBIN	200 µg/kg	ND	145/145	N/A
PARATHION-METHYL	200 µg/kg	ND	145/145	N/A
PERMETHRIN TRANS		ND	82.8/82.8	N/A
PIPERONYLBUTOXIDE	2000 µg/kg	ND	145/969	N/A



CHLORANTRANIL-IPROLE	200 µg/kg	ND	145/145	N/A
PYRETHRINS CINERIN I		ND	96.8/96.8	N/A
PYRETHRINS CINERIN II		ND	98.8/98.8	N/A
PYRETHRINS JASMOLIN I		ND	78.5/78.5	N/A
PYRETHRINS JASMOLIN II		ND	61.0/61.0	N/A
PYRETHRINS PYRETHRIN I		ND	451/451	N/A
PYRETHRINS PYRETHRIN II		ND	266/266	N/A



RESULTS CERTIFIED BY:  
BARRY CHAFFIN  
COO, NOVA ANALYTIC LABS  
MAR 03, 2023

RESULTS CERTIFIED BY:  
GREG NEWLAND  
CSO, NOVA ANALYTIC LABS  
MAR 03, 2023

RESULTS CERTIFIED BY:  
CHRIS ALTOMARE  
CEO, NOVA ANALYTIC LABS  
MAR 03, 2023

[https://lims.tagleaf.com/coa\\_/1y2Lvs5fXK](https://lims.tagleaf.com/coa_/1y2Lvs5fXK)

\* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OMP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED.

END OF REPORT




## CERTIFICATE OF ANALYSIS

\* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

**H.23.006.BIN-METALS (TINCTURE) // PRODUCED: JUL 25, 2023**

**CLIENT: HEALER HEMP LLC // BATCH: PASS**



**BATCH NO.:** H.23.006 <sup>1</sup>  
**MATRIX:** TINCTURE <sup>1</sup>  
**SAMPLE ID:** NAL-230721-019  
**COLLECTED ON:** JUL 21, 2023  
**RECEIVED ON:** JUL 21, 2023  
**SAMPLE SIZE:** 2.668 G <sup>1</sup>  
**SAMPLED BY:** ANNA KUPEL  
**RECEIVED BY:** IAN LEONARD

<sup>1</sup> ENTERED BY CLIENT



**NOVA ANALYTIC LABS**  
Tomorrow's Testing, Today.

### MANUFACTURER INFO

**MANUFACTURER**  
HEALER HEMP LLC  
119 ORION ST  
BRUNSWICK, MAINE 04011

**LICENSE**  
CGR26424  
MEDICINAL - CAREGIVER

### BATCH RESULT: PASS

**METALS** PASS

**HME.1: HEAVY METALS BY ICP-MS**  
**PREPARATION: JUL 24, 2023 // ANALYSIS: JUL 25, 2023**

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
ARSENIC	1500 µg/kg	ND	10.0/84.1	PASS
CADMIUM	500 µg/kg	ND	4.34/84.1	PASS

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
LEAD	500 µg/kg	ND	4.64/101	PASS
MERCURY	3000 µg/kg	ND	15.5/67.3	PASS



**AUTHORIZED BY:**  
ZACHARY SMITH  
LABORATORY MANAGER, NOVA  
ANALYTIC LABS  
JUL 25, 2023

\* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OCP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED. THIS CERTIFICATE OF ANALYSIS IS RELEVANT ONLY TO THOSE ITEMS TESTED. THE SAMPLE WAS PROVIDED TO THE LABORATORY FOR TESTING BY THE CLIENT AND THE SAMPLE WAS TESTED AS RECEIVED.


**END OF REPORT**

## CERTIFICATE OF ANALYSIS

\* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.

**H.23.006.BIN-PEST (TINCTURE) // PRODUCED: JUL 25, 2023**

**CLIENT: HEALER HEMP LLC // BATCH: PASS**



**BATCH NO.:** H.23.006 <sup>1</sup>  
**MATRIX:** TINCTURE <sup>1</sup>  
**SAMPLE ID:** NAL-230721-018  
**COLLECTED ON:** JUL 21, 2023  
**RECEIVED ON:** JUL 21, 2023  
**SAMPLE SIZE:** 2.688 G <sup>1</sup>  
**SAMPLED BY:** ANNA KUPEL  
**RECEIVED BY:** IAN LEONARD

<sup>1</sup> ENTERED BY CLIENT



**NOVA ANALYTIC LABS**  
 Tomorrow's Testing, Today.

### MANUFACTURER INFO

**MANUFACTURER**  
 HEALER HEMP LLC  
 119 ORION ST  
 BRUNSWICK, MAINE 04011

**LICENSE**  
 CGR26424  
 MEDICINAL - CAREGIVER

### BATCH RESULT: PASS

**PESTICIDES** TESTED

**: PESTICIDES, INSECTICIDES, FUNGICIDES AND GROWTH REGULATORS BY LC-HRMS**  
**PREPARATION: JUL 24, 2023 // ANALYSIS: JUL 24, 2023**


ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
NALED	500 µg/kg	ND	139/186	N/A
OXAMYL	1000 µg/kg	ND	139/465	N/A
PHOSMET	200 µg/kg	ND	139/139	N/A
ACEPHATE	400 µg/kg	ND	139/186	N/A
ALDICARB	400 µg/kg	ND	139/186	N/A
BOSCALID	400 µg/kg	ND	139/186	N/A
CARBARYL	200 µg/kg	ND	139/139	N/A
DIAZINON	200 µg/kg	ND	139/139	N/A
FIPRONIL	400 µg/kg	ND	139/186	N/A
IMAZALIL	200 µg/kg	ND	139/139	N/A
METHOMYL	400 µg/kg	ND	139/186	N/A
PROPOXUR	200 µg/kg	ND	139/139	N/A
SPINOSAD	200 µg/kg	ND	139/139	N/A
ABAMECTIN	500 µg/kg	ND	139/186	N/A
ETOXAZOLE	200 µg/kg	ND	139/139	N/A
MGK-264 I		ND	85.0/85.0	N/A
MALATHION	200 µg/kg	ND	139/139	N/A
METALAXYL	200 µg/kg	ND	139/139	N/A
PYRIDABEN	200 µg/kg	ND	139/139	N/A
BIFENAZATE	200 µg/kg	ND	139/139	N/A
BIFENTHRIN	200 µg/kg	ND	139/139	N/A
CARBOFURAN	200 µg/kg	ND	139/139	N/A
CYFLUTHRIN	1000 µg/kg	ND	139/465	N/A
DAMINOZIDE	1000 µg/kg	ND	139/465	N/A
DICHLORVOS	1000 µg/kg	ND	139/465	N/A
DIMETHOATE	200 µg/kg	ND	139/139	N/A
ETOFENPROX	400 µg/kg	ND	139/186	N/A
FENOXICARB	200 µg/kg	ND	139/139	N/A
FLONICAMID	1000 µg/kg	ND	139/465	N/A
MGK-264 II		ND	54.3/54.3	N/A
METHIOCARB	200 µg/kg	ND	139/139	N/A
ACEQUINOCYL	2000 µg/kg	ND	139/929	N/A

ANALYTE	LIMIT	AMT (µg/kg)	LOD/LOQ (µg/kg)	PASS/FAIL
ETHOPROPHOS	200 µg/kg	ND	139/139	N/A
FLUDIOXONIL	400 µg/kg	ND	139/186	N/A
HEXYTHIAZOX	1000 µg/kg	ND	139/465	N/A
PRALLETHRIN	200 µg/kg	ND	139/139	N/A
SPIROXAMINE	400 µg/kg	ND	139/186	N/A
THIACLOPRID	200 µg/kg	ND	139/139	N/A
AZOXYSTROBIN	200 µg/kg	ND	139/139	N/A
CHLORFENAPYR	1000 µg/kg	ND	139/465	N/A
CHLORPYRIFOS	200 µg/kg	ND	139/139	N/A
CLOFENTEZINE	200 µg/kg	ND	139/139	N/A
CYPERMETHRIN	1000 µg/kg	ND	139/465	N/A
IMIDACLOPRID	400 µg/kg	ND	139/186	N/A
MYCLOBUTANIL	200 µg/kg	ND	139/139	N/A
SPIROMESIFEN	200 µg/kg	ND	139/139	N/A
TEBUCONAZOLE	400 µg/kg	ND	139/186	N/A
THIAMETHOXAM	200 µg/kg	ND	139/139	N/A
FENPYROXIMATE	400 µg/kg	ND	139/186	N/A
PACLOBUTRAZOL	400 µg/kg	ND	139/186	N/A
PROPICONAZOLE	400 µg/kg	ND	139/186	N/A
SPIROTETRAMAT	200 µg/kg	ND	139/139	N/A
PERMETHRIN CIS		ND	59.9/59.9	N/A
KRESOXIM-METHYL	400 µg/kg	ND	139/186	N/A
TRIFLOXYSTROBIN	200 µg/kg	ND	139/139	N/A
PARATHION-METHYL	200 µg/kg	ND	139/139	N/A
PERMETHRIN TRANS		ND	79.4/79.4	N/A
PIPERONYLBUTOXIDE	2000 µg/kg	ND	139/929	N/A

ACETAMIPRID	200 µg/kg	ND	139/139	N/A	CHLORANTRANIL-IPROLE	200 µg/kg	ND	139/139	N/A
					PYRETHRINS CINERIN I		ND	92.8/92.8	N/A
					PYRETHRINS CINERIN II		ND	94.8/94.8	N/A
					PYRETHRINS JASMOLIN I		ND	75.3/75.3	N/A
					PYRETHRINS JASMOLIN II		ND	58.5/58.5	N/A
					PYRETHRINS PYRETHRIN I		ND	432/432	N/A
					PYRETHRINS PYRETHRIN II		ND	255/255	N/A



**AUTHORIZED BY:**  
ZACHARY SMITH  
LABORATORY MANAGER, NOVA  
ANALYTIC LABS  
JUL 25, 2023



*\* FOR QUALITY ASSURANCE PURPOSES. NOT A MAINE COMPLIANCE CERTIFICATE.*

ALL TESTS WERE PERFORMED IN ACCORDANCE WITH THE RULES AND REGULATIONS SET FORTH IN THE MAINE ADULT USE PROGRAM. LABORATORY SAMPLING PROTOCOLS ARE GOVERNED BY THE OCP'S SAMPLING GUIDANCE DOCUMENTS. ALL INFORMATION PROVIDED BY THE CLIENT, INCLUDING SELF SAMPLING, MUST BE ACCURATE AND ADHERE TO THE SAME RULES AND REGULATIONS. HOWEVER, CLIENT PROVIDED INFORMATION, INCLUDING SAMPLING, IS ULTIMATELY THE RESPONSIBILITY OF THE PROVIDING LICENSEE, REGISTERED CAREGIVER, PATIENT OR THE LIKE AND FAILURE TO FOLLOW SAID PROTOCOLS COULD LEAD TO ERRONEOUS TEST RESULTS. NOTE: NOT ALL POTENTIAL AND/OR EXISTING HAZARDS WERE ANALYZED. THIS CERTIFICATE OF ANALYSIS IS RELEVANT ONLY TO THOSE ITEMS TESTED. THE SAMPLE WAS PROVIDED TO THE LABORATORY FOR TESTING BY THE CLIENT AND THE SAMPLE WAS TESTED AS RECEIVED.

**END OF REPORT**

